

karma

User manual

Evo Lectus Low Rider

■ Lectus Seat (EVO-LTS-LR)



A Better Wheelchair, A Better Fit

Contents



NOTE

- Product availability may vary by country/region. Visit www.karmamedical.com or contact your local sales representative for details.
- Standard features and available options may differ depending on regional market specifications. Please refer to the configuration of the product as purchased.

1. How to contact KARMA	1
2. Declaration of Conformity	2
3. Introduction	6
3.1 Chassis number	6
4. Used symbols for warning, caution, and note	8
5. Warranty	9
6. Intended use/intended user	10
7. Intended environment	11
8. Tire pressure	11
9. The wheelchair	12
9.1 Parts description of Evo Lectus Low Rider (EVO-LTS-LR)	12
9.2 Chassis	14
9.2.1 Chassis suspension	14
9.2.2 Tie-down loops	15
9.2.3 Lights and reflectors	15
9.2.4 Battery compartments	16
9.2.5 Main fuse	18
9.2.6 Seat lift (Optional)	19
9.2.7 Seat height	20

9.3 Seat	20
9.3.1 Upholstered seat cushion	21
9.3.2 Seat rail	21
9.3.3 Seat tilt (Optional)	22
9.3.4 Upholstered backrest	23
9.3.5 Power recline backrest (Optional)	23
9.3.6 Upholstered armrest	24
9.3.7 Legrest	24
9.3.8 Powered legrest adjustment (Optional)	25
9.3.9 Support wheels	26
9.3.10 Upholstered headrest (Optional)	26
9.3.11 Upholstered calf support (Optional)	27
9.3.12 Upholstered lateral support (Optional)	28
9.3.13 Upholstered hip support (Optional)	28
9.3.14 Pelvic positioning belt	29
9.4 Controls	29
9.4.1 Side steering control	29
9.4.2 Tray table control (Optional)	30
9.4.3 Attendant control (Optional)	30
9.5 Other options/accessories	31
10. First set up	32
10.1 Chassis suspension	32
10.1.1 Spring setting	32
10.1.2 Damper setting	34
10.2 Seat adjustments	35
10.2.1 Seat depth	35
10.2.2 Seat width	38

10.2.3 Armrest width	40
10.2.4 Armrest height	44
10.2.5 Armrest angle	45
10.2.6 Armrest depth	46
10.2.7 Armrest inside angle	47
10.2.8 Legrest length	48
10.2.9 Legrest angle	49
10.2.10 Footplate angle	50
10.2.11 Calf support settings	51
10.2.12 Headrest settings	53
10.2.13 Hip support settings	55
10.2.14 Lateral support settings	59
10.3 Pelvic positioning belt	60
10.4 Control settings	61
10.4.1 Height adjustment side control:	61
10.4.2 Depth adjustment side control	62
11. Control panel	62
11.1 Charging socket	62
11.2 Joystick	63
11.3 Display	63
11.3.1 Battery indicator (top bar)	63
11.3.2 Focus light (top bar)	64
11.3.3 Profile name (main screen)	64
11.3.4 Clock (main screen)	64
11.3.5 Speed display (main screen)	65
11.3.6 Speed bar (main screen)	65
11.3.7 Inhibit (main screen)	65

11.3.8 Seat functions (main screen)	66
11.3.9 Additional options (main screen)	66
11.3.10 Message screen (main screen)	66
11.3.11 Current profile (base bar)	68
11.3.12 Motor temperature (base bar)	68
11.3.13 Control system temperature (base bar)	68
11.3.14 Wheelchair lock	68
11.4 Buttons	71
11.4.1 On/Off button	71
11.4.2 Horn button	71
11.4.3 Speed decrease button	71
11.4.4 Speed increase button	72
11.4.5 Mode button	72
11.4.6 Profile button	72
11.4.7 Hazard Warning Button and LED	72
11.4.8 Lights Button and LED	72
11.4.9 Left Indicator Button and LED	73
11.4.10 Right Indicator Button and LED	73
11.5 Jack sockets	73
11.5.1 External profile switch jack	73
11.5.2 External on/off switch jack	74
11.6 R-net Connectors	74
11.7 Joystick	75
12. Electric system	76
12.1 Batteries	76
12.2 Fuses	77
13. Using the wheelchair	79

13.1	General warnings and advices _____	79
13.2	Use in combination with other products _____	80
13.3	Hot and cold surfaces _____	81
13.4	Danger of pinching _____	81
13.5	Surroundings _____	82
13.6	Precautions to prevent dangerous situations _____	82
13.7	Use on slopes: driving on downhill slopes _____	84
13.8	Use on slopes: driving on uphill slopes _____	86
13.9	Driving on sideways slopes _____	87
13.10	Obstacle climbing _____	88
13.11	Use in presence of electromagnetic fields, e.g. from cell phones _____	89
14.	Driving the wheelchair _____	91
14.1	Driving in general _____	91
14.2	Driving technique _____	93
14.3	Stopping the wheelchair _____	93
15.	Using the powered seat functions _____	94
15.1	Seat lift _____	95
15.2	Seat tilt _____	96
15.3	Backrest _____	97
15.4	Legrest _____	98
15.5	Support wheels _____	99
15.6	Relax position _____	100
15.7	Negative tilt _____	101
15.8	PRO-Motion function _____	102
15.9	Using additional function of the wheelchair menu _____	104
16.	Handling the mechanical brakes _____	105
16.1	Release the mechanical brakes _____	105

17. Charging the maintenance-free batteries _____	106
17.1 Battery level _____	106
17.2 Charging socket _____	108
17.3 Disposal of broken or worn-out batteries _____	109
18. Transport of the wheelchair _____	110
18.1 4-point tie down restraint system _____	110
18.1.1 Transportation guideline _____	112
18.1.2 Safety belt _____	114
18.2 Transportation using Dahl Docking station _____	118
18.2.1 Mounting of the Dahl locking adapter on the wheelchair _____	119
18.2.2 Locking procedure: _____	124
18.2.3 Unlocking procedure: _____	124
18.2.4 Manually unlocking in case of electric failure or accident: _____	125
18.2.5 Safety belt _____	126
18.3 Transportation on an airplane _____	129
18.3.1 Batteries _____	129
18.3.2 The wheelchair's dimensions and weight _____	129
19. Maintenance and repairs _____	130
19.1 Battery charging _____	130
19.2 Short-term storage _____	130
19.3 Long-term storage _____	131
19.4 Tools _____	132
19.5 Wheels and tires _____	133
19.5.1 Puncture repair _____	133
19.6 Cleaning _____	135
19.6.1 Upholstery, cloth/airmesh _____	135
19.6.2 Metal surfaces _____	135

19.6.3 Plastic covers	136
19.7 Brake release, freewheel mode	136
19.8 Battery replacement	137
19.9 Replacing the main fuse	139
20. Refurbishment and re-use of the product.	140
21. Disposal of the product	141
22. Troubleshooting	141
22.1 Diagnostics R-net LCD	142
23. Safety information	144
24. Technical specifications	145
25. Accessories	150

1. How to contact KARMA

Karma

Head office

KARMA Medical

Address: No. 2363, Sec. 2, University Rd., Min-Hsiung Shiang,
Chia-Yi 621, Taiwan

Phone: +886 5 206 6688

Email: globalsales@karma.com.tw

Website: www.karmamedical.com

European representative

KARMA Mobility S.L.

Address: C/ Periodista Francisco Carantoña Dubert,
23 Bajo 33209 Gijón - Asturias (Spain)

Phone: +34 984 390 907

Email: karma@karmamobility.es

Website: www.karmamobility.es

UK representative

KARMA Mobility Ltd.

Address: Unit 6 Target Park, Shawbank Road, Redditch,
B98 8YN England United Kingdom

Phone: +44 845 630 3436

Email: info@karmamobility.co.uk

Website: www.karmamobility.co.uk



Produced and published by KARMA Medical, Taiwan
Technical changes and print errors prohibited.

2. Declaration of Conformity



Document No.: DOC-EU-Evo Lectus LR-03

EU Declaration of Conformity

We, with the information specified in the below,

Our information as the manufacturer:

Manufacturer's Name:	KARMA MEDICAL PRODUCTS CO., LTD
Manufacturer's Address:	NO. 2363, Sec. 2, University Rd., Min-Hsiung Shiang, Chia-Yi County, 62144, Taiwan
SRN (Single Registration Number):	TW-MF-000013206

Our authorized representative:

Name:	KARMA MOBILITY, S.L.
SRN (Single Registration Number):	ES-AR-000004852
Address:	C/ PERIODISTA FRANCISCO CARANTOÑA DUBERT, 23 Bajo 33209 GIJÓN – ASTURIAS, SPAIN
Contact Person:	Raquel Yuste
Contact Information:	(+34) 984 390 907

in accordance with

Regulation (EU) 2017/745 of the European Parliament and of the council Annex I, II, III, IV and IX

hereby declare that the medical device specified below:

Basic UDI-DI of Annex VI:	471987385EvoXC
Device:	Electrically powered wheelchair
Trade Name or Mark:	Evo Lectus Low Rider
Model Number:	EVO-LTS-LR
Product Code according to EMDN:	Y122127
Product Code according to GMDN:	41875
Classification:	Rule 13 of Class I
UDI-DI:	04719873856893

is in conformity with the applicable requirements of the following documents:

Ref. No.	Title	Edition date
ISO 13485	Medical devices - Quality management systems - Requirements for regulatory purposes	2016
ISO 14971	Medical devices - Application of risk management to medical devices	2019
EN 12182	Assistive products for persons with disability - General requirements and test methods	2012
EN 12184	Electrically powered wheelchairs, scooters and their chargers - Requirements and test methods	2014
EN 62366	Medical devices - Application of usability engineering to medical devices	2015
EN 60601-1	Medical electrical equipment - Part 1: General requirements for basic safety and essential performance	2006
EN ISO 10993-1	Biological evaluation of medical devices - Part 1: Evaluation and testing within a risk management process	2009
EN ISO 10993-5	Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity	2009
EN ISO 15223-1	Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied - Part 1: General requirements	2016
MEDDEV. 2.7/1 Rev. 4	CLINICAL EVALUATION: A GUIDE FOR MANUFACTURERS	2016
MEDDEV 2.12/1 Rev. 8	GUIDELINES ON A MEDICAL DEVICES VIGILANCE SYSTEM	2013

The information on this declaration has been stated on the sole responsibility of KARMA MEDICAL PRODUCTS CO., LTD.

We hereby declare that the device named above has been designed to comply with the relevant sections of the above referenced specifications. The device complies with all General Safety and Performance Requirements.

Intended purpose: The wheelchair is intended to provide mobility for individuals with limited mobility

Date of issue: 9th September 2025

Place of issue: NO. 2363, Sec. 2, University Rd., Min-Hsiung Shiang, Chia-Yi County, 62144, Taiwan


CHEN, YING-CHUN CEO

UK Declaration of Conformity

We, with the information specified in the below,

Our information as the manufacturer:

Manufacturer's Name:	KARMA MEDICAL PRODUCTS CO., LTD
Manufacturer's Address:	NO. 2363, Sec. 2, University Rd., Min-Hsiung Shiang, Chia-Yi County, 62144, Taiwan
SRN (Single Registration Number):	TW-MF-000013206

Our UK responsible person:

Name:	Karma Mobility Ltd
MHRA Reference Number:	11480
Address:	Unit 6 Target Park, Shawbank Road, Redditch, B98 8YN England United Kingdom
Contact Person:	Mr Mark Duffield
Contact Information:	01527 520 468

in accordance with

UK MDR 2002 and Council Directive 93/42/EEC concerning medical devices in

Annexes I, II and VII hereby declare that the medical device specified below:

Basic UDI-DI of MDR (Annex VI):	471987385EvoXC
Device:	Electrically powered wheelchair
Trade Name or Mark:	Evo Lectus LR
Model Number:	EVO-LTS-LR
Product Code according to EMDN:	Y122127
Product Code according to GMDN:	41875
Classification:	Rule 13 of Class I
UDI-DI:	04719873856893

is in conformity with the applicable requirements of the following documents:

Ref. No.	Title	Edition date
EN ISO 13485	Medical devices - Quality management systems - Requirements for regulatory purposes	2016
EN ISO 14971	Medical devices - Application of risk management to medical devices	2019
EN 12182	Assistive products for persons with disability - General requirements and test methods	2012
EN 12184	Electrically powered wheelchairs, scooters and their chargers - Requirements and test methods	2014
EN 62366	Medical devices - Application of usability engineering to medical devices	2015
EN 60601-1	Medical electrical equipment - Part 1: General requirements for basic safety and essential performance	2006
EN ISO 10993-1	Biological evaluation of medical devices - Part 1: Evaluation and testing within a risk management process	2009
EN ISO 10993-5	Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity	2009
EN ISO 15223-1	Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied - Part 1: General requirements	2016

The information on this declaration has been stated on the sole responsibility of KARMA MEDICAL PRODUCTS CO., LTD.

We hereby declare that the device named above has been designed to comply with the relevant sections of the above referenced specifications. The device complies with all Essential Requirements.

Intended purpose: The wheelchair is intended to provide mobility for individuals with limited mobility

Date of issue: 9th September 2025

Place of issue: NO. 2363, Sec. 2, University Rd., Min-Hsiung Shiang, Chia-Yi County, 62144, Taiwan


CHEN, YING-CHUN CEO

3. Introduction

Congratulations on your new KARMA product! This product has been made with great care and dedication. The KARMA product will increase your freedom of mobility and independence. KARMA and its resellers all over the world are there to support in any way. So, if you have questions or suggestions about our products, do not hesitate to get in contact with us at globalsales@karma.com.tw

Before you use the KARMA product, we strongly recommend you read this manual carefully and always keep it with your product. This way you are always able to find additional information when needed.

KARMA runs the policy of continuous product improvement. Therefore, the actual appearance of the products or options might be different from the pictures shown in this manual. KARMA reserves the right to make changes to the product without prior notice.

3.1 Chassis number

The chassis number is very important. Your wheelchair will be stored in our data system under this main number. You can find the number on the rear end of the chassis.



Chassis serial plate

The symbols used on the chassis plate are explained below:



This icon describes the model and type of the product.



This icon stands for indoor- and outdoor use (Class B).



This icon stands for the date of production.



This icon stands for the maximum driving speed.



This icon stands for the maximum slope to drive on.



This icon stands for the maximum user weight.

SN:

This icon stands for the chassis serial number.



WARNING

- The wheelchair is designed for a maximum user weight of 136 kg. Avoid reading the inappropriate load labeling as it could lead to overloaded usage.
- Avoid incomplete labeling.

4. Used symbols for warning, caution, and note

General admonitions are indicated by a symbol. There are three levels of admonition.

- **Warning**



WARNING

If you see this sign, please use extreme caution where this symbol appears. Neglecting these warnings can lead to personal or material damage.

- **Caution**



CAUTION

If you see this symbol, use caution to prevent dangerous situations.

- **Note**



NOTE

If you see this symbol, we provide additional information which might be good to know. Please take notice of this information.



NOTE

- Do not install, maintain or operate the wheelchair without reading this manual. That is, before using the wheelchair, you should read this manual to get familiar with this product.
- Make sure the local reseller has set up the product in a proper way to exactly fit your needs and requirements.
- Always be accompanied by an attendant when you drive the wheelchair for the first time.



NOTE

- The first drive should take place in a safe and wide area, so you can get acquainted with your wheelchair without any danger.
- Always start to drive the wheelchair at the lowest possible driving speed first.

5. Warranty

KARMA Medical supplies a warranty of frame for a period of 5 years and electrical system (controller, motor, charger, actuator, and PCB) for a period of 1 year after delivery to the customer. Your local supplier will carry out this warranty. For battery warranty, it is subject to the periods set by the manufacturers. Please contact your local supplier in detail.

For a warranty claim, you get in contact with our local authorized KARMA reseller or directly with KARMA Mobility S.L. Make sure you also provide the chassis serial number of your product. The wheelchair must be repaired by a KARMA Medical designated Customer Service agent. This warranty is VOID if the original chassis serial number is removed or altered.

The warranty does not apply to damage or faults of the product caused by wrong or improper use, or neglected maintenance. The evaluation of it is the privilege of KARMA Medical or a representative to be appointed by KARMA Medical.

This guarantee does not apply to components susceptible to wear, such as bearings, cables, carbon brushes, circuit breakers, covers, footplates, light bulbs, pads, side guards, upholsteries, wheels, and similar parts.

The warranty does not cover any consequential costs arising from the rectification of defects, including but not limited to freight and travel expenses, labor charges, service fees, or any transportation costs for repair or replacement.

KARMA Medical reserves the right to alter the specifications at any time. No responsibility can be accepted for any changes in the specifications.

Change of specification can be originated from e.g. availability of parts, product improvement based on market experience, changed legislations, etc.



WARNING

- The use of non-original parts on this product can lead to personal or material damage. KARMA Medical cannot be held responsible for these results.
- Repairs executed by unauthorized persons can lead to personal or material damage. KARMA Medical cannot be held responsible for these results.



NOTE

If you have any doubt about the service provided to your wheelchair, please contact KARMA Medical Taiwan for information.

6. Intended use/intended user

The Evo Lectus Low Rider (EVO-LTS-LR) powered wheelchair is meant to provide mobility to persons who are not able to walk, stand or use a manual wheelchair, but who are very well able to control and use the interface of a powered wheelchair. The wheelchair is designed for a maximum user weight of 136 kg.

Apart from the horizontal mobility, the Evo Lectus Low Rider (EVO-LTS-LR) provides the user with mobility in vertical direction. This includes to reach light switches, a doorbell or doorknobs.

It is strongly suggested to have the use of the wheelchair evaluated by a trained doctor, therapist or other qualified and trained staff.

This wheelchair is not suitable for persons who do not have the cognitive skills to drive a powered wheelchair by themselves. Also, it is not suitable for visually impaired persons.

The expected service life of the product is **5 years**, presuming that the product is used daily in accordance with the safety operation instructions, inspection and maintenance instructions, and intended use, which are described in this manual.

7. Intended environment

The Evo Lectus Low Rider (EVO-LTS-LR) powered wheelchair is not restricted to only indoor or only outdoor use. Because the large driving wheels are placed in the front, the wheelchair is extremely maneuverable and is able to cope with many terrain differences. This, combined with the compact size of the Evo Lectus Low Rider (EVO-LTS-LR) and the excellent speed range and battery capacity, making the wheelchair suitable for both indoor and outdoor use.

It is allowed to use the wheelchair in different weather conditions. It can be used at temperatures of -25 degrees up to maximum 55 degrees Celsius. However, it must be noticed that metal or plastic surfaces of the wheelchair can become very hot when exposed to direct sun for longer time.

Because of the harmful combination of saltwater and sand, it is advised not to use the wheelchair on beaches. We advise to clean the wheelchair after having been in contact with sand and/or saltwater as described in the "Cleaning" section.

8. Tire pressure

The Evo Lectus Low Rider (EVO-LTS-LR) uses air-filled (standard) or solid (optional) tires in the front and in the rear. The choice of having air-filled or solid tires is made by the user during the ordering of the wheelchair. In order to prevent tire damage and to preserve the performance of the wheelchair, the tire pressure must be checked at least on a monthly basis. The tire pressure should be:

Drive wheel air-filled tires: max. 300 Kpa/43.5 PSI/3 bar


Rear caster air-filled tires: max. 200 Kpa/29.0 PSI/2 bar

9. The wheelchair

9.1 Parts description of Evo Lectus Low Rider (EVO-LTS-LR)



- | | |
|----------------------------|-----------------------------|
| 1. Headrest | 8. Rear caster |
| 2. Backrest | 9. Drive wheel |
| 3. Pelvic positioning belt | 10. Front battery box |
| 4. Seat | 11. Front caster |
| 5. Armrest | 12. Footplate |
| 6. Tie-down loops | 13. Calf support |
| 7. Front light/Turn signal | 14. Central mounted legrest |
| | 15. Controller |

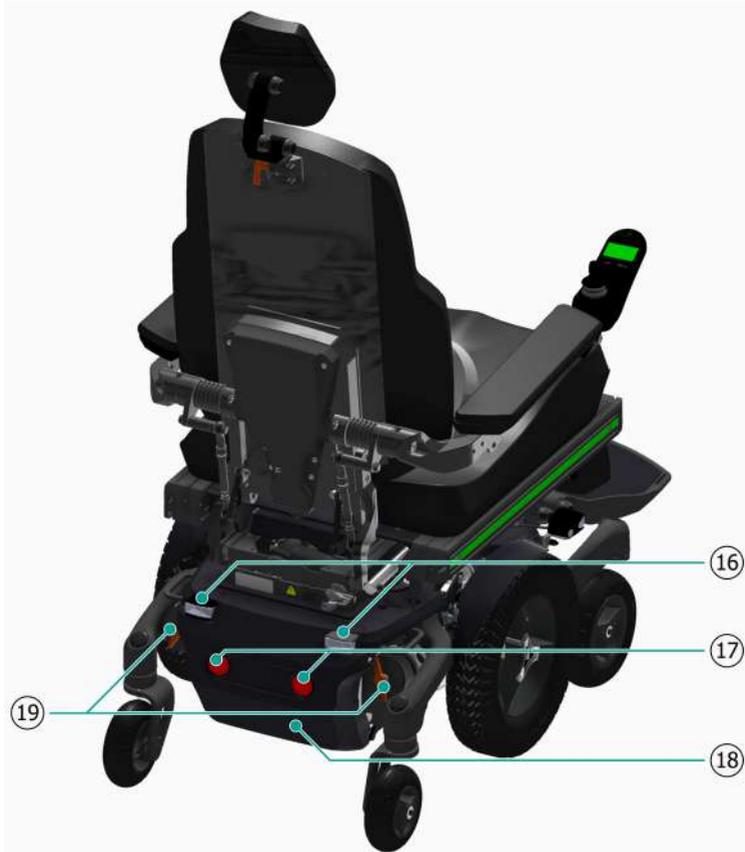

16. Rear lights/Turn signals

17. Reflectors

18. Rear battery box

19. Freewheel switches

9.2 Chassis

The chassis is the base of the wheelchair. It contains wheels, drive motors, batteries, electronics and seat lift. The steel parts of the chassis are electrolytic anodized and powder coated to ensure a long life without corrosion.



Each of the drive wheels is propelled by a powerful drive motor. These motors also take care of the steering of the wheelchair. With this system, it is possible to turn on the spot. This makes the wheelchair optimal for indoor use.

9.2.1 Chassis suspension

The chassis has independent suspension on each of the four wheels. The stiffness can be adjusted to your personal requirements.




Front suspension



Rear suspension

9.2.2 Tie-down loops

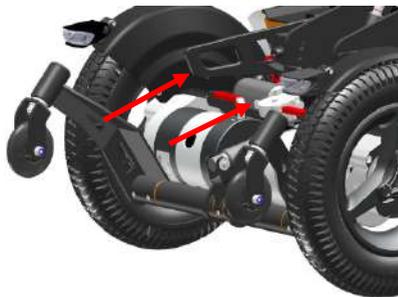

Tie-down loops in the front





Tie-down loops in the rear

The tie-down loops are marked with this sign:
Further information about transportation of the wheelchair you will find in chapter "transportation".



9.2.3 Lights and reflectors

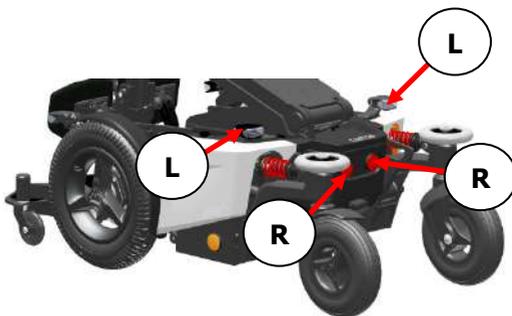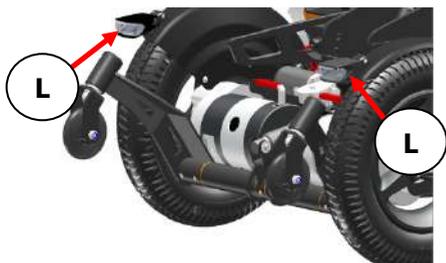

The chassis has very strong and bright LED lights to make sure you can have a safe drive in the dark. The orange reflectors on both sides and the red reflectors on the rear also make you visible to other people as well. The lights fulfill the European requirements. (E marked)

The additional LED indicators give our environment clear information in which direction you want to go.

9.2.4 Battery compartments


The batteries are mounted as low as possible and as central as possible into the chassis to provide an optimal center point of gravity. This results in a maximum stability of the wheelchair. The compartment can hold maintenance-free batteries up to 85Ah. For the specification of the batteries see the chapter technical specifications.

The maintenance-free batteries can be reached from the side. They can be replaced whilst the user is still in the wheelchair.



The battery box


To reach the batteries, first remove the locking bolt [A]. Lift up the plastic cover vertically [B], then pull it off the chassis in the horizontal direction [C].

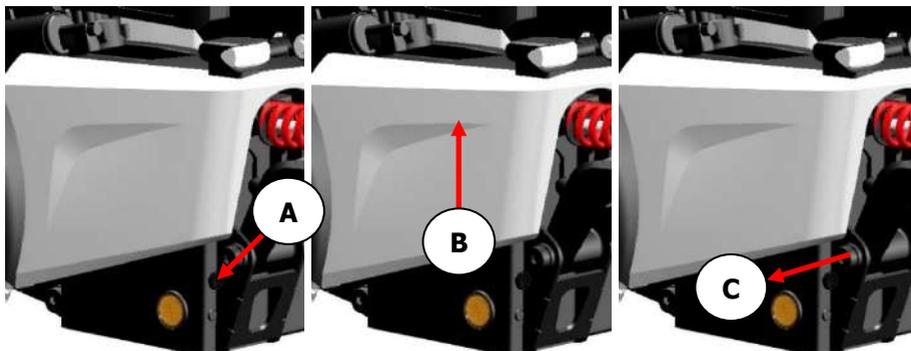

After taking the cover off, the maintenance-free battery can be pulled out of the box.


Mind the cables!

At installing the maintenance-free battery, one should pay great attention to make sure the cables are not jammed between the battery and the battery box.

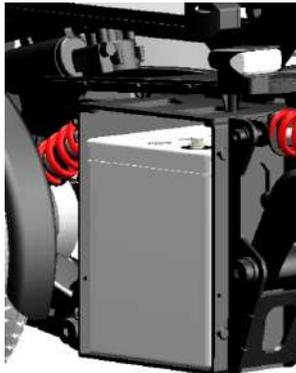

CAUTION

- When pulling the battery out of the box do mind to not overstretch the cables. This might lead to technical failure.
- Before removing the batteries, first remove the main fuse. This is to reduce the risk of short circuit or electrical shock. See the chapter of the main fuse.
- Before reconnecting the battery, read the wiring instructions on the inside of the battery cover.

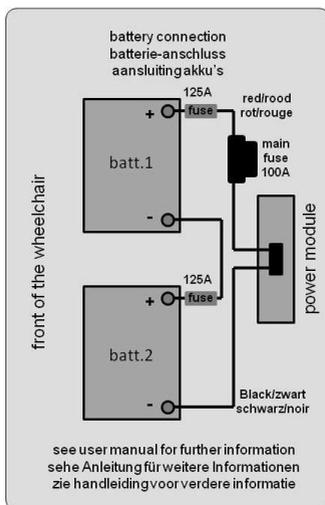

9.2.5 Main fuse

The chassis contains a main fuse which is located at the rear of the chassis.



Position of the main fuse



Main fuse

The main fuse protects the whole electrical system of the wheelchair. This fuse will only blow if there is a serious problem on the wheelchair.



CAUTION

If the main fuse has blown, do not replace the fuse immediately. First contact your local supplier to have the wheelchair checked.

The fuse also works as a main switch. By removing the main fuse the batteries are disconnected. This is important when the wheelchair is transported in an airplane. To remove the fuse, simply pull the plastic cover off and pull the fuse.




CAUTION

Only use original main fuses as replacement. Using other fuses might lead to material damage to the wheelchair.

9.2.6 Seat lift (Optional)

The seat lift is centrally mounted into the chassis. With this lift the seat can be raised stepless up to 400 mm. This enables the user to have more freedom of movement, not only in horizontal area, but also in the vertical area. The seat lift can be stopped at any height and will be automatically locked in position.

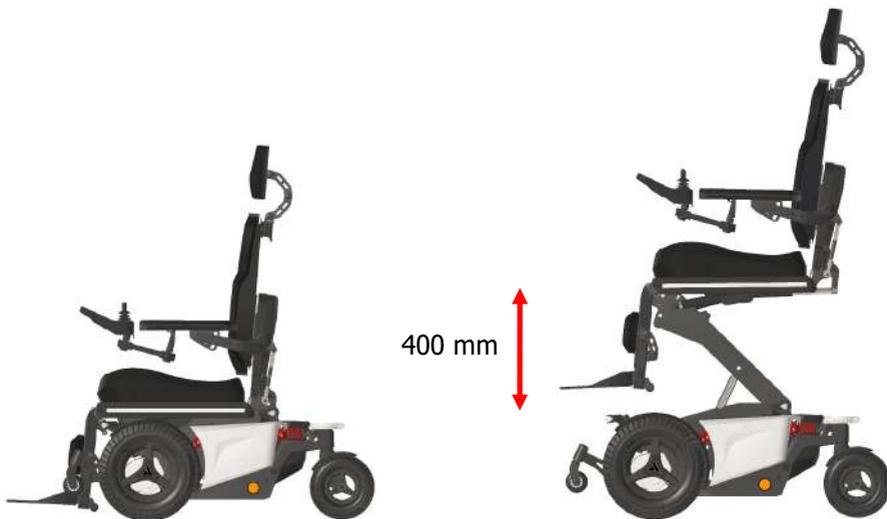

Whilst lifting the seat, the driving speed will automatically reduce to gain maximum stability at all times. At high seating position also the seat tilt will be blocked to gain maximum stability. The seat height can be set to every height position by the user. The maximum seat height is set to 865 mm (seat pan to ground).



CAUTION

Be careful driving in high seating position at slopes. We strongly suggest to only use the seat lift on flat areas. Lifting high on a steep slope might lead to instability and might cause personal or material damage.



NOTE

The seat lift can also be very helpful for transferring or lifting the user in or out of the wheelchair.

9.2.7 Seat height

The lower seat frame is centrally mounted into the chassis. There are several pre-adjusted seat height options possible. The lowest seat height from floor to seat pan is 415 mm. This can be pre-adjusted in increments of 10 mm until a maximum seat height of 465 mm.



NOTE

The setting of the seat height has direct influence on the ground clearance of the legrests.

9.3 Seat

The seating system is designed to optimize the seating comfort to the user. It can be adjusted in seat depth and seat width. A rail on each side provides mounting point for accessories like hip supports or safety belts. The seat pan is flat so other seating cushion can be fitted on to the seat as well.



9.3.1 Upholstered seat cushion

The upholstered seat cushion is available in different sizes to provide optimal seating comfort and support to the user. The cloth is available as airmesh or breathing but waterproof cloth. The seat cushion is well fixed with Velcro on to the seat pan to prevent it from sliding.



NOTE

Using other cushions with different thickness might influence the biomechanical function of the legrest and or backrest.

9.3.2 Seat rail

On each side of the seat frame there is a rail to mount different accessories to the wheelchair. The middle area can be personalized with a color sticker.



Seat rail

9.3.3 Seat tilt (Optional)

The seat tilt can be used to release pressure. The tilting angle is from 0 to 45°. The tilt can also be used when driving down a slope for compensating the negative seat angle. This provides a more stable seat position and safe driving.



If the tilt is activated over a certain angle, the driving speed will be reduced. This is to reduce the risk of danger whilst driving at high speed.



CAUTION

- Always drive carefully on slopes. The angle of the slope has great influence on the total stability of the wheelchair.
- When tilting always check if there are no obstructions close to the wheelchair. Especially in the front or rear of the wheelchair.
- When tilting, the wheelchair will get longer. This has influence on the driving characteristics of the wheelchair. Make sure there is enough space to drive.

9.3.4 Upholstered backrest

The upholstered backrest is available in different lengths and width sizes to give the users maximum support and comfort. The cloth is available as airmesh or breathing but waterproof cloth.

9.3.5 Power recline backrest (Optional)

The power recline backrest can be set from 85° to a flat horizontal position. It gives the user the possibility to move into a laying position or a very active sitting position.



At a reclined backrest position over 135°, the driving speed will be automatically reduced for safety reasons.



CAUTION

- When reclining always check if there are no obstructions close to the wheelchair. Especially in the rear of the wheelchair.
- When reclining, the wheelchair will get longer. This has influence on the driving characteristics of the wheelchair. Make sure there is enough space to drive.
- Always drive carefully on slopes. The angle of the slope has great influence on the total stability of the wheelchair.

9.3.6 Upholstered armrest

The upholstered armrests of the seat provide good and comfortable support of the arm which result in a stable seating position. The armrest has a soft upholstery on the top side. The arm rests come in 320 mm or 400 mm length.

A biomechanical mechanism makes sure the armrests are always in a good position to supply optimal support.

The armrests are adjustable in height, depth, angle and inside angle. For transferring in and out of the chair, the armrests can be flipped up.



9.3.7 Legrest

The legrest uses a central mounted tube on which the footplates are mounted. The footplates come in two different sizes. The legrest can be adjusted in length (left and right footplate independent) knee angle and footplate angle (left and right independent). The footplates can be flipped up to decrease the size of the wheelchair for transportation or storage. A build in rail can be used to mount calf supports.

9.3.8 Powered legrest adjustment (Optional)

With a powered legrest the knee angle can be set from little less than 90° up to a fully stretched leg angle. The biomechanical mechanism ensures the lower leg length will always be the same.




If the legrest is stretched over 45° the driving speed will automatically be reduced for safety reasons.



CAUTION

- When stretching the legrest always check if there are no obstructions close to the wheelchair. Especially in the front of the wheelchair.
- When stretching the legrest, the wheelchair will get longer. This has influence on the driving characteristics of the wheelchair. Make sure there is enough space to drive.

9.3.9 Support wheels

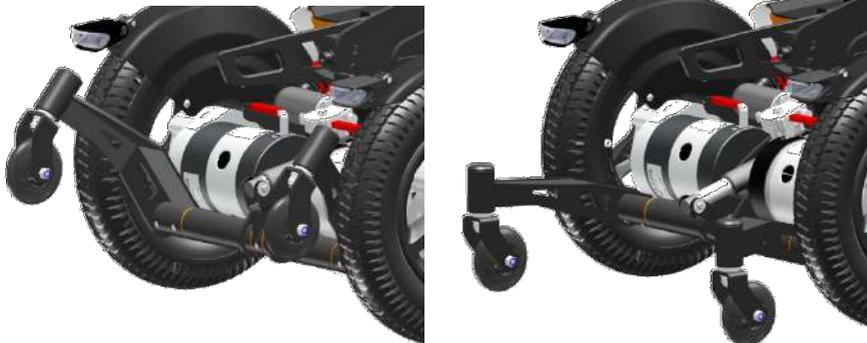

The support wheels prevent the wheelchair tipping over when moving when moving into the vertical position. The support wheels are positioned in front of the drive wheels and are automatically activated by the electronic system.

Driving in slow speed is still possible in case the support wheels are activated and touch the ground.



WARNING

Only drive in standing position if the wheelchair is on a horizontal and flat surface.

9.3.10 Upholstered headrest (Optional)

The upholstered headrest is adjustable in height, depth and angle to the requirements of the user. It can be taken off without losing its settings.

As an additional option, a rail can be mounted to move the headrest out of center. Another option is a rotation block to rotate the headrest to the left or right.





NOTE

If the wheelchair user is transported in a taxi van we strongly advise to use the headrest. This is in order to provide you optimal stability whilst driving in the taxi.

9.3.11 Upholstered calf support (Optional)

The upholstered calf supports are adjustable in height, depth, width and angle. They give additional support when using a powered legrest.



9.3.12 Upholstered lateral support (Optional)

The optional upholstered lateral support offer support on the upper body. The supports are adjustable in height, width, depth and angle. The supports can also be flipped sideways for transferring in or out of the wheelchair. During this sideways flipping the adjustments stay intact. The soft rounded pads ensure optimal support and great comfort.



9.3.13 Upholstered hip support (Optional)

The upholstered hip supports offer side support to your hips or upper leg. The support is adjustable in height, depth, width and angle. The soft pads offer good and comfortable support.




The hip supports can be taken away for transferring in or out of the wheelchair, without losing the settings.

9.3.14 Pelvic positioning belt

For positioning, several types of belts are available.



(Optional)

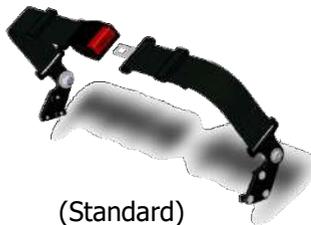

(Standard)



NOTE

The pelvic positioning belt shall not be used as a car safety belt. If transported in a car, the user needs to wear an additional car safety belt.

9.4 Controls

9.4.1 Side steering control



side steering, fixed bracket



side steering, swing-away (Optional)



The Evo Lectus Low Rider (EVO-LTS-LR) wheelchair has a side steering control unit, which is either mounted on the left- or right armrest. The joystick module can be mounted on a fixed bracket or on an (optional) swing away mechanism. This system enables you to sit close to a table.

9.4.2 Tray table control (Optional)



Tray table control, driving position *Tray table control, flipped over*

The tray table control enables the user to have a table with a center mounted built-in joystick module. The table can be flipped up sideways for transferring in and out of the wheelchair. The joystick module can be flipped over to use the table as desktop. When flipped over, the driving mode of the wheelchair is automatically blocked. This ensures safe use of the wheelchair in any position.

9.4.3 Attendant control (Optional)



The attendant control enables the user to have a handle with a built-in joystick module. The attendant control can be arranged on the left or right side of the back plate.

9.5 Other options/accessories

Item	Figure	Introduction
Center Mount One-piece Footplate		To provide a lower footplate with respect to the ground and to provide a comprehensive support plane with the support weight up to 136 kg.
Armrest support		Could be arranged on the armrest to support the weight up to 136 kg on single side.
Tray table Universal		To provide a desktop for user when head or leg controller is used.
Bumper wheels		To prevent collision of the case and rear casters when moving backward.
Warning light		To provide the warning and direction light in front and back.



CAUTION

The arrangement of the options/accessories should take the motion of wheel and cables into consideration. It is suggested to set up those options/accessories by an authorized KARMA supplier

10. First set up

Before using, the wheelchair needs to be adjusted and set up for the user. In this chapter we will explain all the setup which needs to be done before the first drive.




CAUTION

Before using the wheelchair it is vital to make the right set up for the user. A non-proper set up of the wheelchair might lead to uncontrolled driving which can result in personal or material damage.

10.1 Chassis suspension

The suspension of a chassis has been designed to increase the comfort whilst driving. Also climbing steps will be easier having suspension on the chassis. But suspension can also be a disadvantage. A suspension which is set to soft has a negative influence on the control of the wheelchair. So, it is very important to have a good mix.

10.1.1 Spring setting

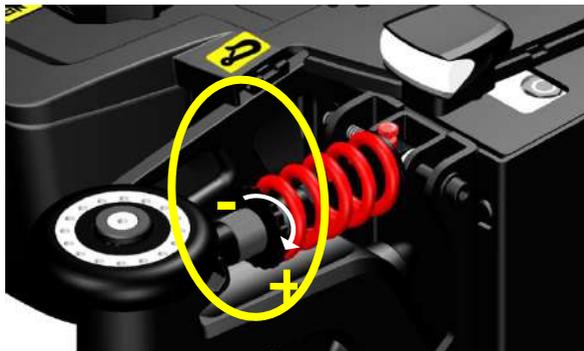

The strength of the spring will be set by turning the ring shown above. By turning it to the right (clockwise) the spring will have more tension and the chassis becomes stiffer. This increases mechanical traction and improves control. The stiffness of the suspension depends on the user weight. The setting needs to be done by setting and testing. We advise you to start with a

stiffer setting, since this results in the best control. If the suspension is too hard, you can set it softer by turning the ring more counter clockwise. To make sure the balance of the left and right spring is the same, we need to measure the setting.



The best way is to measure the distance between the ring and the end of the tread in mm. Make sure that the spring settings in the front are identical. The same for the two rear springs.



CAUTION

- To soft settings of the spring will result in a very spongy behavior of the chassis. The control of the wheelchair will be bad. Avoid soft settings.
- If the springs are uneven set, it might lead to strange driving behavior of the wheelchair. This might result in personal or material damage.



NOTE

After setting the suspension, always drive first slowly and in an open space to test the result of the setting.

10.1.2 Damper setting

The spring damper unit has a red adjustment wheel on the end of the damper. This wheel adjusts the rebound speed of the spring.



Turning the red knob clockwise will make the movement of the piston going out again faster. This decreases the damping of the spring damper unit. Turning the knob counter clock wise will increase the damping. The right setting will be done by stetting and testing whilst driving. The average setting is halfway. This is set by counting the clicks from the totally left position to the totally right setting. These are 16 clicks. Now set the setting by 8 clicks form the end position.



CAUTION

- To soft settings of the damper will result in a very spongy behavior of the chassis. The control of the wheelchair will be bad. Avoid soft settings.
- If the dampers are uneven set, it might lead to strange driving behavior of the wheelchair. This might result in personal or material damage.



NOTE

After setting the suspension, always drive first slowly and in an open space to test the result of the setting.

10.2 Seat adjustments


Before using the wheelchair, the seat must be set to the right size for the user. Most of the time this will be done by your local supplier, together with your therapist. A well-adjusted seat will give you optimum support and comfort. Especially the bio-mechanical adjustment is based on a well-adjusted seat size.

10.2.1 Seat depth

To adjust the seat depth, take the following steps:

Step 1: Pull off the seat cushion.

Step 2: Loosen the top seat panel screws (A) using a 3 mm Allen key.

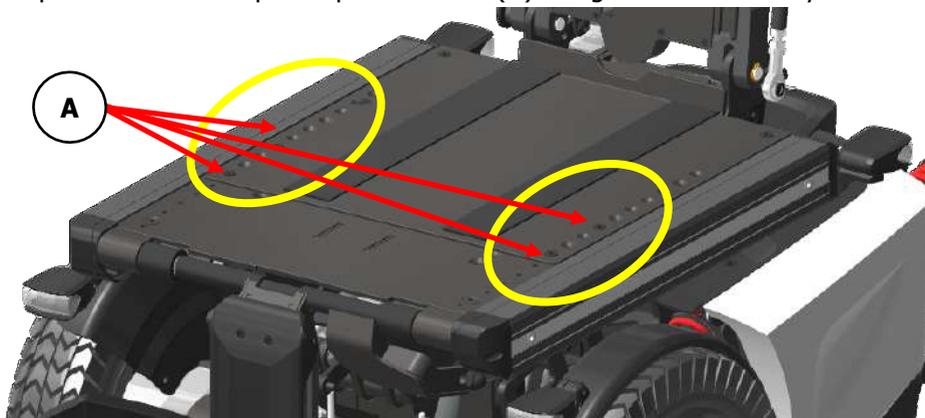


Step 3: Take off the top seat panel.


Step 4: Loosen the screws (**B**) of the side rails using an Allen key size 4 mm.
And take the side rail away.



Step 5: Loosen the screws (**C**) of the backrest sliding unit using a 5 mm Allen key.

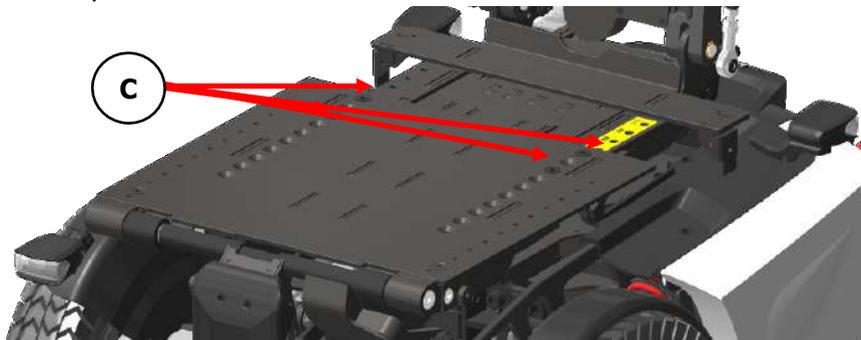

Step 6: Move the backrest frame backward to increase the seat depth or
forwards to reduce the seat depth.

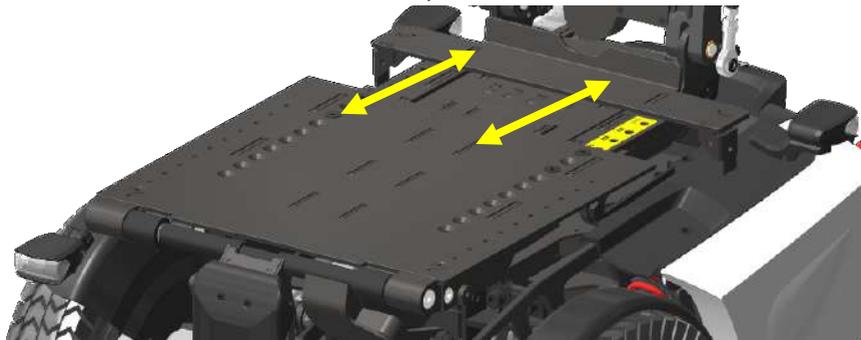

The seat depth is adjustable in steps of 25 mm, starting at a seat depth of 400 mm.




NOTE

The setting of the seat depth requires some expertise. Therefore we strongly advise you to have it done by your local authorized KARMA dealer.

Step 7: Tighten the screws of the backrest frame and fixate the adjustment tube to fixate the seat depth.


Step 8: Mount the side rails into position and tighten the bolts (**D**).

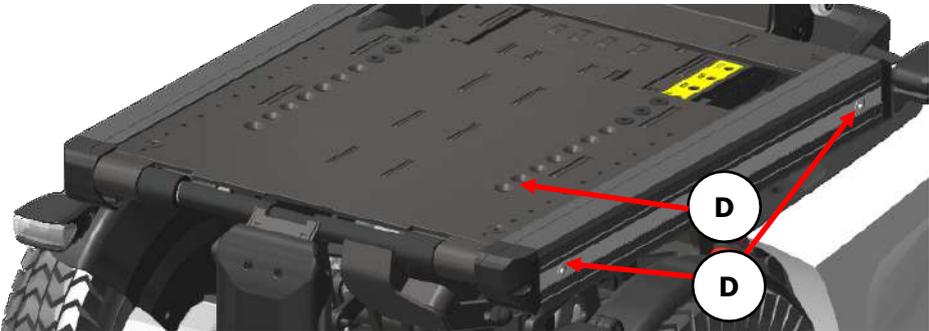

NOTE

With every seat depth comes a different length of seat rail. Pre-order the right length of rail first before changing the seat depth.

Step 9: Place the top seat panel back into position and tighten the screws (E).

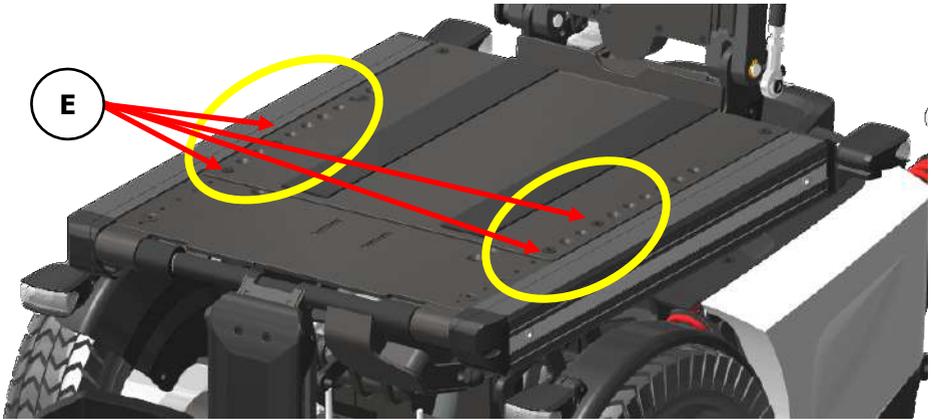

Now, the seat cushion can be put back into place.




10.2.2 Seat width

To increase the seat width, additional extension rail can be mounted. Please take the following steps to increase the seat width:



Step 1: Take off the cushion.

Step 2: Loosen the screws of the side rail (**F**) and remove them.

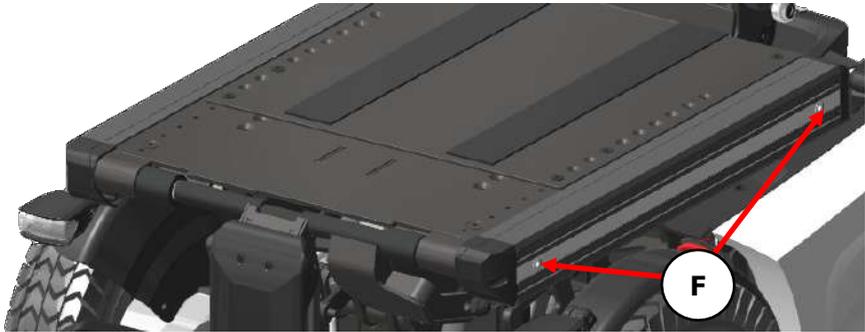

Step 3: Unpack the additional extension rail.



Step 4: Place the extension rail into position and place the longer mounting bolts which came with the extension rail.




Step 5: Tighten the bolts and place the wider seat cushion on the seat pan.


10.2.3 Armrest width

The distance between both armrests can be changed in steps by 50 mm. To change the distance, take the following steps:


Step 1: Remove the rear cover of the backrest. To do this, you must use a 3 mm Allen key to loosen the 6 small screws.

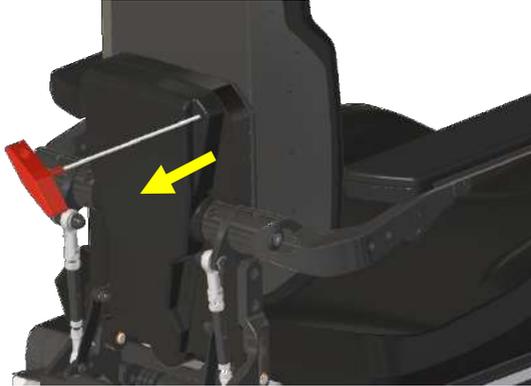

Step 2: Loosen and remove the two bolts using a 5 mm Allen key.

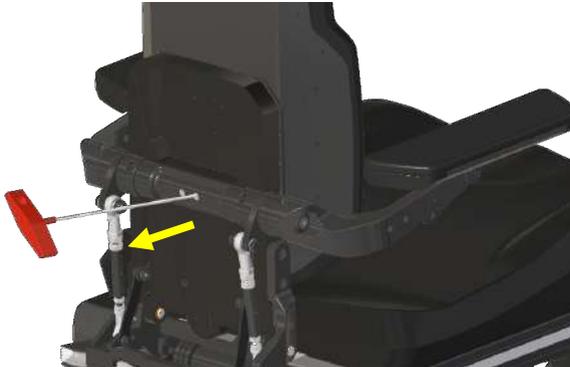

Step 3: Remove the bolts and detach the parallel bar from the armrest.

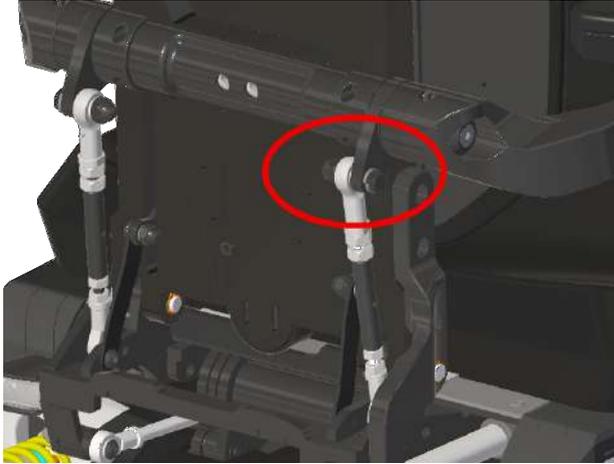


CAUTION

If the parallel bar is removed, the armrest will fall down. So before removing the parallel bar, make sure you hold the armrest with one hand whilst removing the parallel bar with the other hand.

Step 4: Pull out the armrest axle.




Step 5: Take off the bearing ring (G).

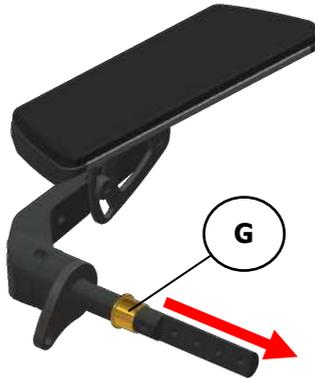


Step 6: Add or remove the spacer of the axle and put the bearing back.



Step 7: Put the axles back into the backrest frame and tighten the two central bolts.

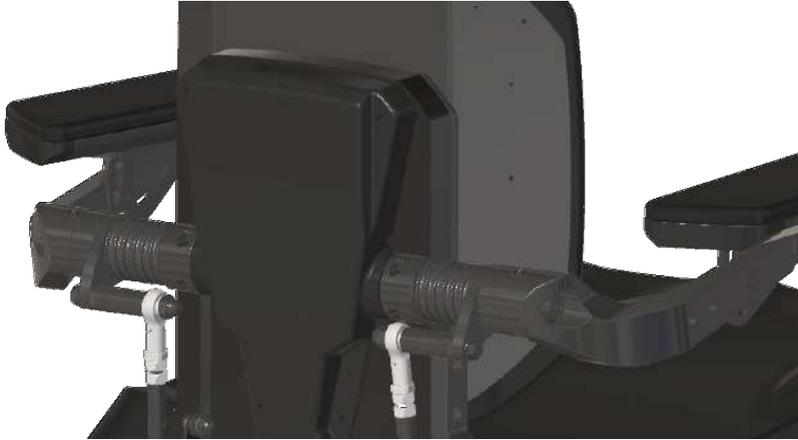

Step 8: Connect both parallel bars and secure them with the locking pin.

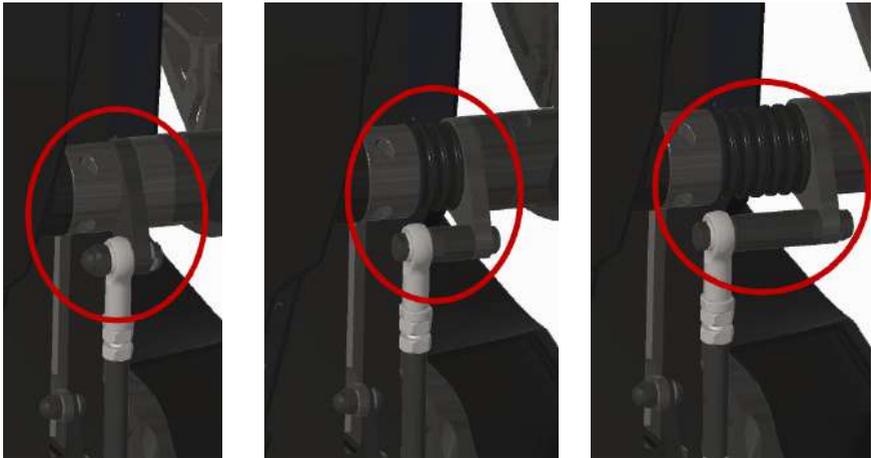


Step 9: Put the backrest cover back on the frame.

Now the armrests are set in to a different width position.


10.2.4 Armrest height

The armrest height can be adjusted up and down independently. To set the right armrest height, take the following steps:

Step 1: Release the locking bolts (**H**) on each side of the armrest using a 5 mm Allen key.

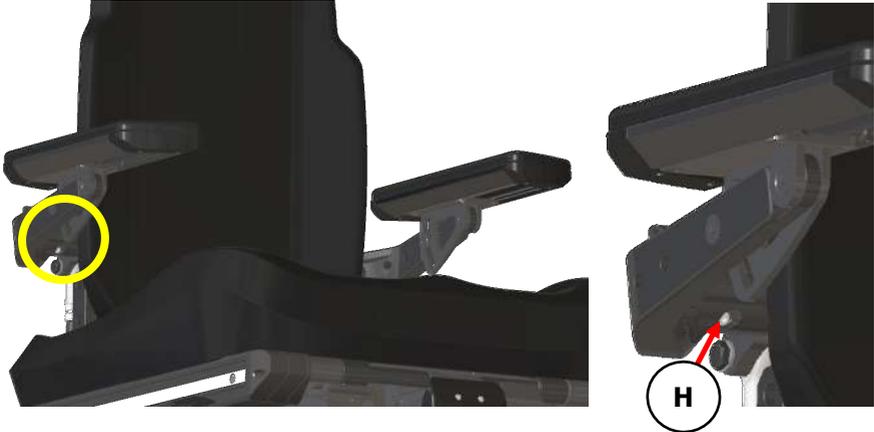

Step 2: Set the armrest angle by using a 5 mm Allen key. By rotating it clockwise the armrest height will increase. By rotating it counterclockwise the armrest height will be reduced.

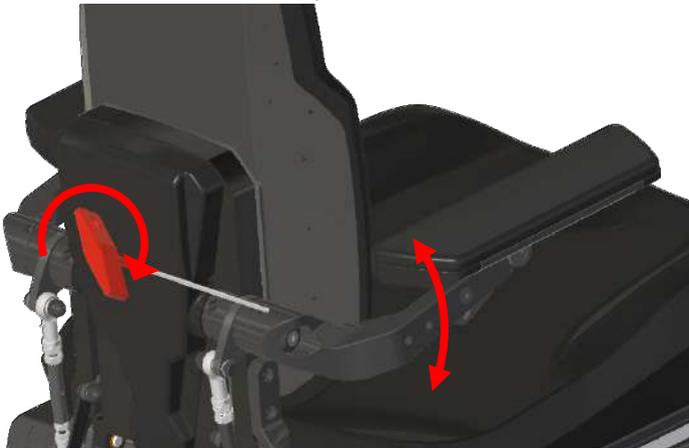


Step 3: Once the right height is set, fixate this position by tightening the locking bolts again.


10.2.5 Armrest angle

To set the right armrest angle, take the following steps:

Step 1: Loosen the front armrest bolt (I) using a 5 mm Allen key. Don't take it out, just loosening.

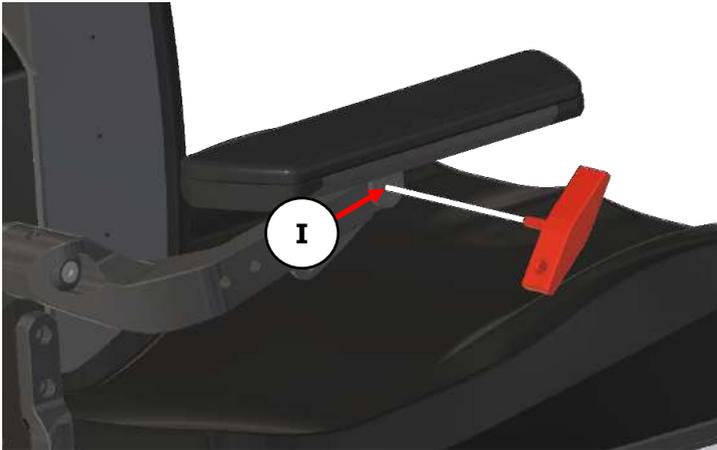

Step 2: Loosen the bolt (J) slightly until the armrest starts to move.

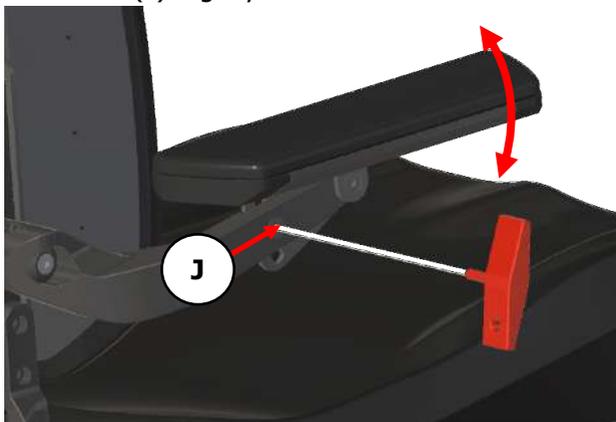



CAUTION


If the second bolt is loosened the armrest will fall down. So loosening the second bolt, make sure you hold the armrest with one hand whilst loosening the bolt with the other hand.

Step 3: Once the right armrest angle is set, first tighten the bolt (**J**) and then the bolt (**I**).

10.2.6 Armrest depth

The armrest can be stepless adjusted in depth. To set the right armrest depth, take the following steps:

Step 1: Loosen the four bolts (**K**) using a 3 mm Allen key.

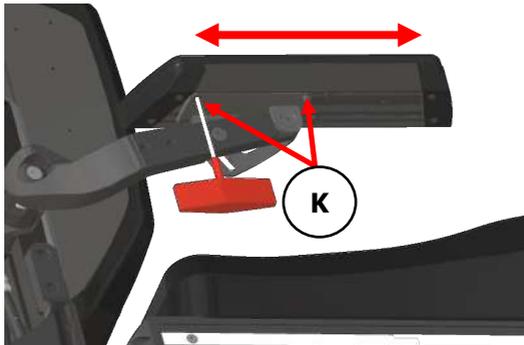


Step 2: Slide the armrest backward or forwards into the required position.

Step 3: Tighten the four bolts. The armrest is set.

10.2.7 Armrest inside angle

The armrest pad can be sideways adjusted over an angle of 15 degrees. To set the armrest inside angle, take the following steps:

Step 1: Loosen the nut (**L**) underneath the armrest pad using a 10 mm wrench head.

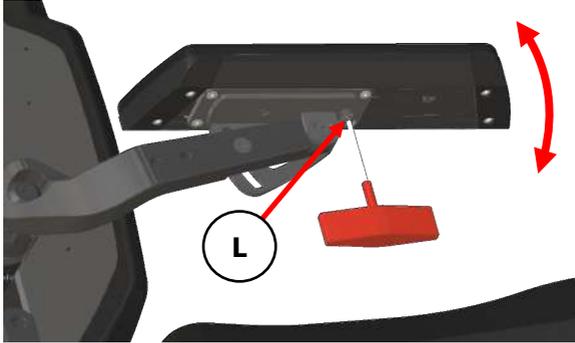

Step 2: Turn the armrest in the required side angle.

Step 3: Tighten the nut again. Now the angle is set.




CAUTION

Always make sure the nut is correctly tightened. Especially on the armrest where the joystick module is mounted. If the armrest is not fixed, it might move whilst driving the wheelchair.

10.2.8 Legrest length

The legrest length is stepless adjustable. Both left and right length is separately adjustable. To set the right length, take the following steps:

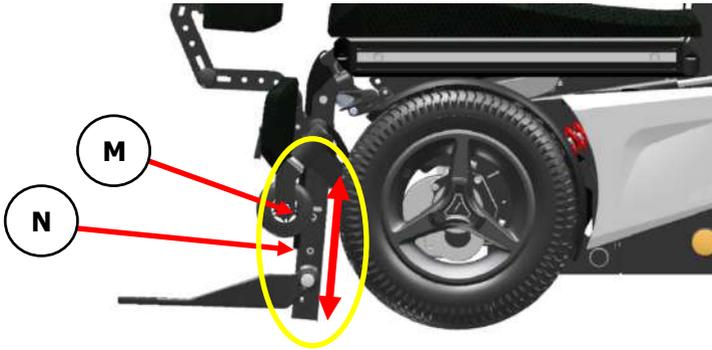

Step 1: Loosen the bottom legrest (**M**) bolt first using a 5 mm Allen key.

Step 2: Slowly loosen the top end bolt (**N**). Just enough to feel the footplate is starting to move.



CAUTION

- By loosening the second bolt on the footplate, the footplate might suddenly start to slide down. If the user has his or her foot on the footplate, this sudden movement might cause a shock reaction. It is best to hold the footplate with one hand and loosen the bolt with the other hand.
- User should be aware of the collision when footplates are set in low or high position. A very low/high footplate should cooperate with specific settings especially when standing function is used. Before adjusting the footplate, please contact authorized supplier.

Step 3: Now slide the footplate into the required position.



NOTE


Make sure the legrest is in the right position. The surface pressure on the upper leg part should be equally divided over the total length. A too short or too long adjusted length might lead to pressure points on the upper legs part.

Step 4: If the right length is set, tighten the bolts firmly.

10.2.9 Legrest angle

The legrest angle can be mechanically set following the next steps:

Step 1: Loosen the bolt (O) on the telescopic tube of the legrest using a 5 mm Allen key. Just open it far enough so you feel it is starting to move.

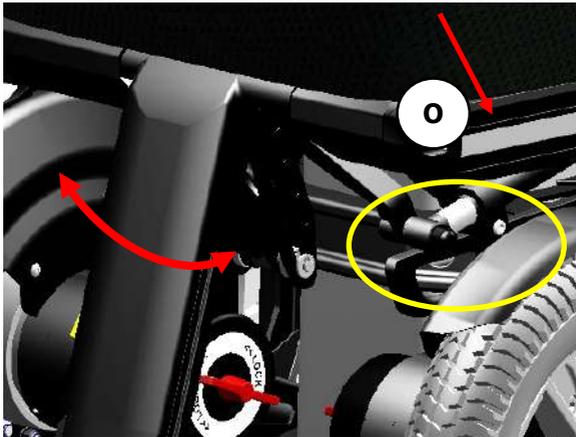

CAUTION

By loosening the bolt of the telescopic tube, the legrest might suddenly start to move down. If the user has his or her feet on the legrest, this sudden movement might cause a shock reaction.

It is best to hold the legrest with one hand and loosen the bolt with the other hand.

Step 2: Move the legrest into the required angle.

Step 3: Tighten the bolt so the setting is fixed.


The legrest angle can optionally be power adjusted. For more information about how to control the powered legrest, refer to the "Using the powered seat functions" chapter.

10.2.10 Footplate angle

The footplate angle can be adjusted for the left and right footplate separately. The setting is stepless. To adjust the angle follow the next steps:

Step 1: Insert the 4 mm Allen key into the adjustment screw inside the footplate.

Step 2: Turn the Allen key clockwise to decrease the angle between footplate and legrest. Turn the Allen key counterclockwise to increase the angle.

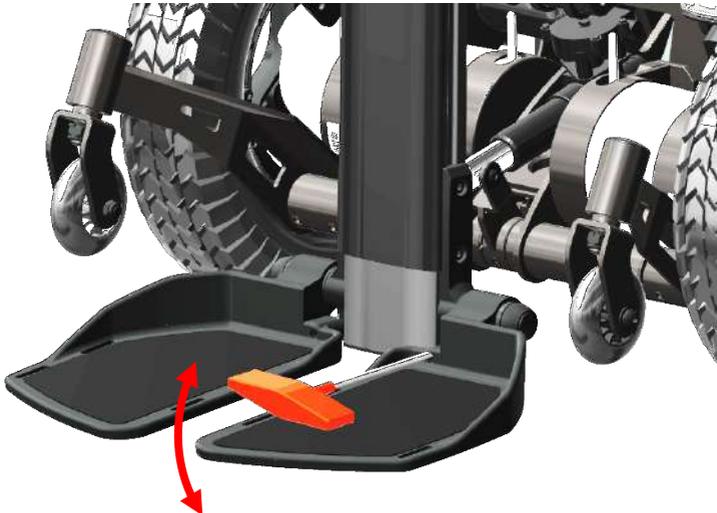




NOTE

The adjustment screw is added with some Loctite to prevent it from moving by itself. For that reason, the turning might a little heavier than expected.

10.2.11 Calf support settings

Optionally, calf supports can be mounted on the legrest. The calf supports are fully stepless adjustable.


10.2.11.1 Adjusting the height of the calf support

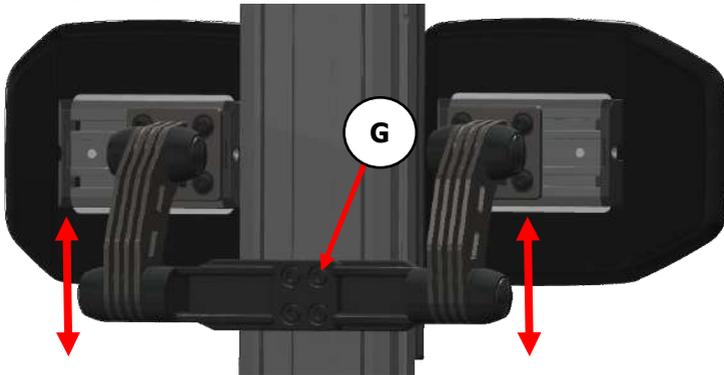

Step 1: Loosen the four bolts (**G**) using a 5 mm Allen key, until the calf support starts to slide in the rail.

Step 2: Slide the calf support into the required height position and fasten the four bolts.

10.2.11.2 Adjusting the width of the calf supports.

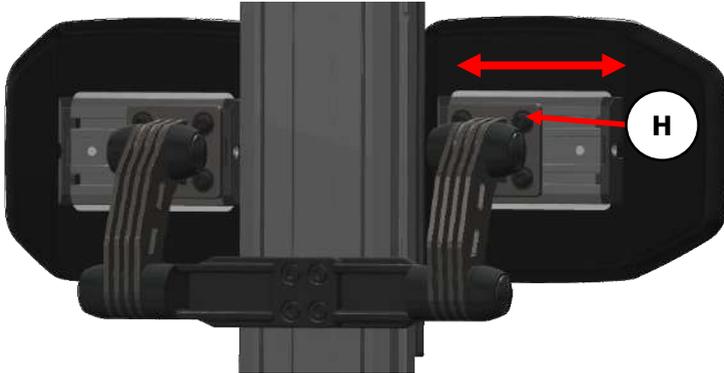


Step 1: Loosen the four bolts (**H**) of the calf support pad using a 5 mm Allen key.

Step 2: Slide the pad into the right position on the rail.

Step 3: Tighten the four bolts. Repeat the same for the other calf support pad.

10.2.11.3 Adjusting the depth and angle of the calf support pads.

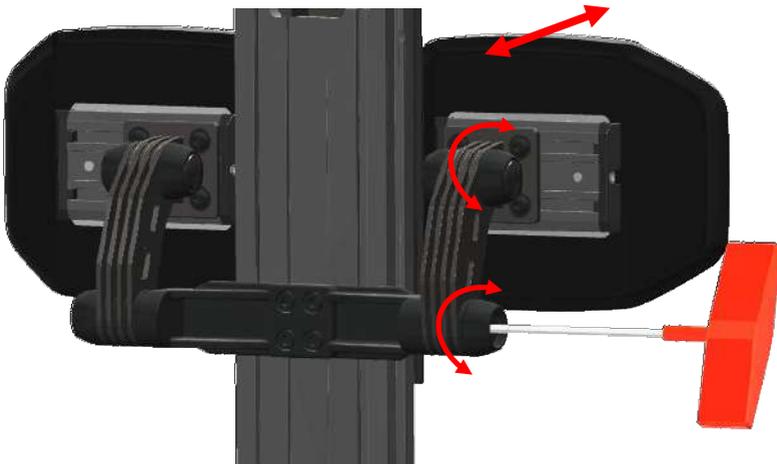

Step 1: Remove the two covers on each side of the calf support.

Step 2: Loosen the bolts of the friction setting using a 6 mm Allen key.


Step 3: Now push the calf support pad in the right depth and angle setting.

Step 4: Tighten the bolts again to fixate the position.

Step 5: Place the covers back onto the friction end caps.


10.2.12 Headrest settings

The optional head rest is fully stepless adjustable to suit the user's needs. It can be taken off without losing its setting.

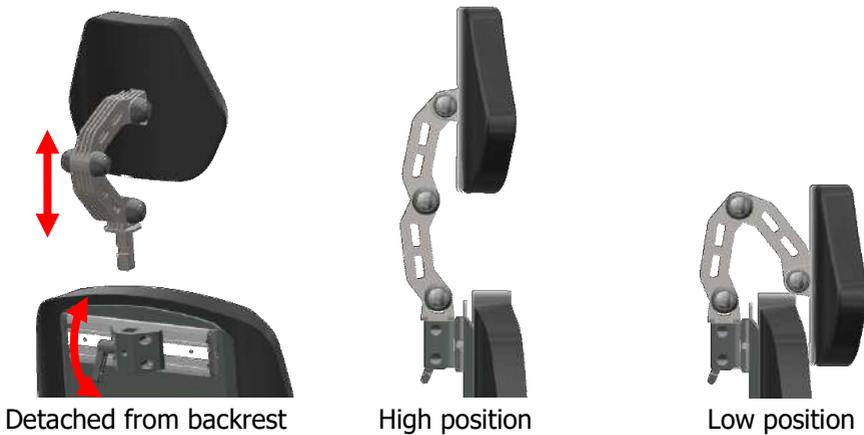

10.2.12.1 Sideways adjustment headrest

The headrest has an optional rail for a sideways off center adjustment. To set this adjustment, take the following steps:

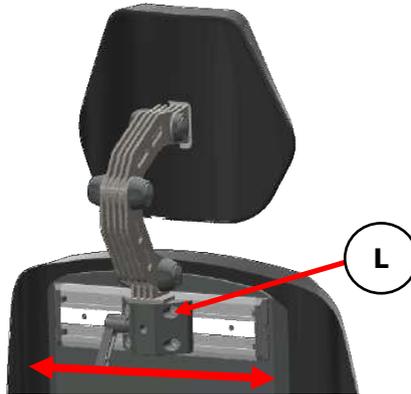


Step 1: Loosen the 4 bolts (L) using a 5 mm Allen key.

Step 2: Move the headrest along the rail into the required position.


Step 3: Tighten the bolts again to fixate the position.

10.2.12.2 Headrest depth, height and angle adjustment.

The headrest has a friction system containing three rotation joints. By moving each rotation joint you can set the height, depth and angle of the headrest all at the same time. To set the headrest in its right position, follow the next steps:

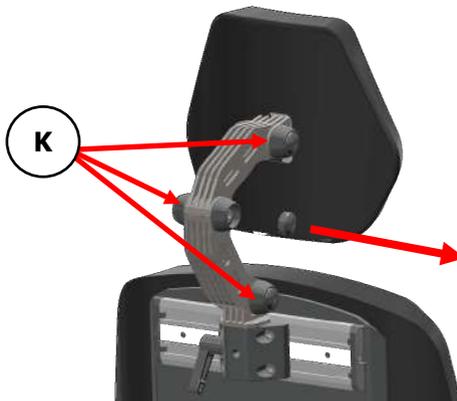

Step 1: Take off the rubber covers (K) of the three joints

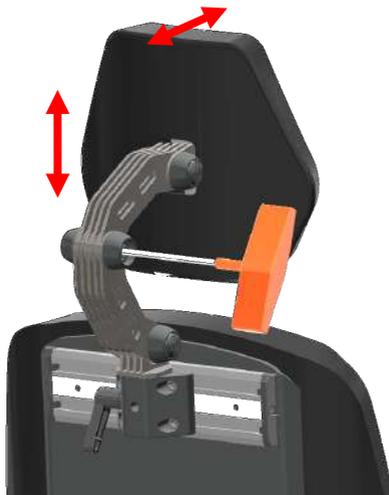

Step 2: Loosen the bolts using a 6 mm Allen key. Loosen then up until the headrest can be moved.

Step 3: Push the headrest into the required position.

Step 4: Tighten the bolts firmly so the position is fixed.

Step 5: Put the rubber covers back on the joints.



CAUTION


If you loosen the bolts too much, the headrest will fall down. This might cause a little shock reaction on the user in the wheelchair. It is better to loosen the bolts bit by bit and every time try to move the headrest. The friction will keep it stable. Make sure you hold the headrest with one hand and loosen the bolt with the other hand.

10.2.13 Hip support settings

The optional hip supports are fully stepless adjustable in side position, height, depth and angle. They can easily be taken off the chair using a quick release system, without its settings.

10.2.13.1 Set the side position on the seat rail

To set the position on the seat rail, take the following steps:

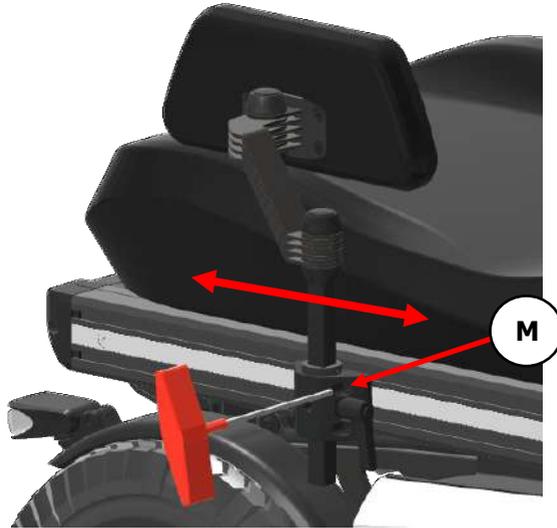


Step 1: Loosen the four bolts (**M**) using a 5 mm Allen Key.

Step 2: Move the hip support into the required position.


Step 3: Tighten the four bolts, the setting is now fixed.

10.2.13.2 Setting the height, width and angle of the hip support

To set the height of the hip support, take the following steps:

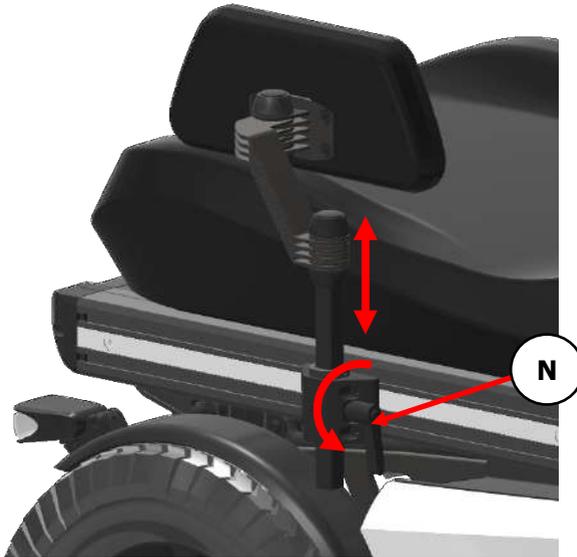


Step 1: Loosen the lever knob (**N**) and lift up the hip support into the right height position.

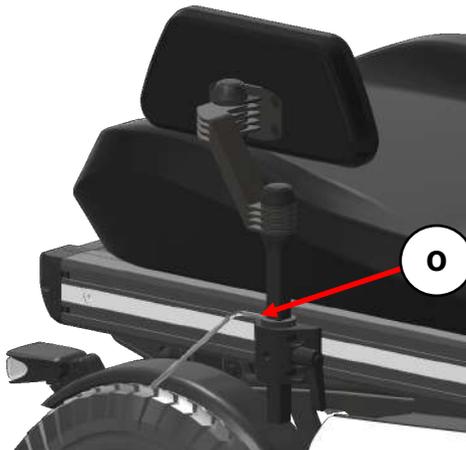


Step 2: Loosen the bolt (**O**) of the fixation ring using a 4 mm Allen key and reposition this ring against the mounting block as a stopper.

Step 3: Tighten the nut of the fixation ring. Now the height is set and secured.

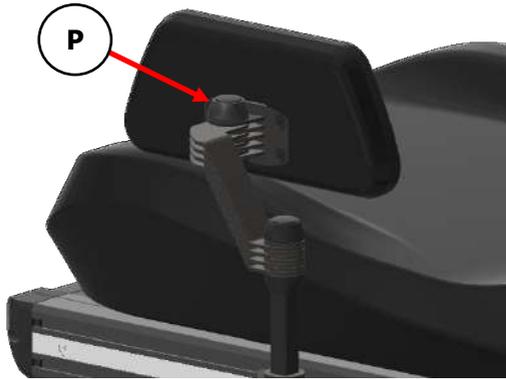

Step 4: Remove the rubber covers (P) of the friction joints.

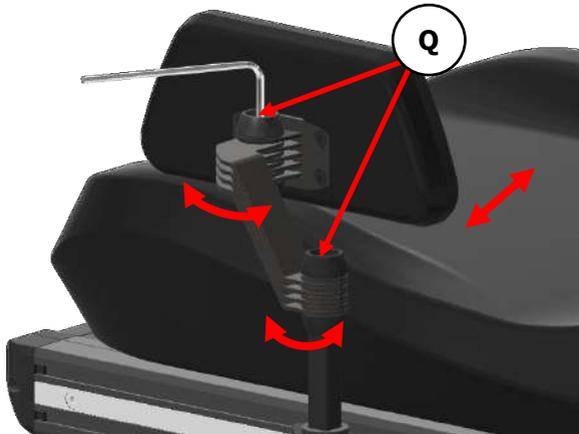

Step 5: Loosen the 2 friction bolts (Q) so the padding can be moved.

Step 6: Tighten the frictions bolts. Now the position is fixed.

Step 7: Put the covers back on to the friction joints.




CAUTION

If you loosen the bolts too much, the hip support might start to suddenly move. This might cause a little shock reaction on the user in the wheelchair. It is better to loosen the bolts bit by bit and every time try to move the hip support pad. The friction will keep it stable. Make sure you hold the hip support with one hand and loosen the bolt with the other hand.

10.2.14 Lateral support settings

The optional lateral support can be adjusted stepless in height, depth, width and angle.

10.2.14.1 Set the height of the lateral support

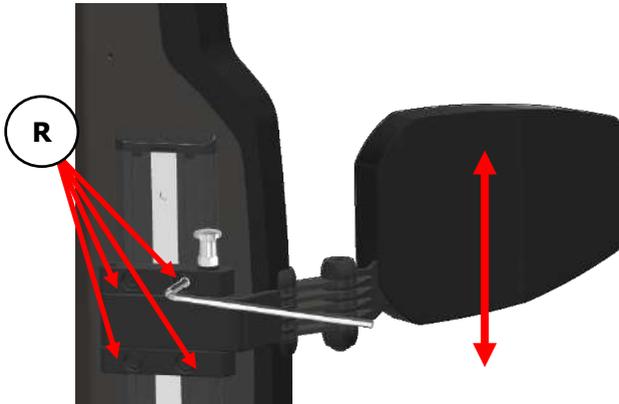


Step 1: Loosen the 4 bolts (**R**) using a 5 mm Allen key.

Step 2: Move the lateral support into the required height.

Step 3: Tighten the bolts.

10.2.14.2 Adjust the depth width and angle of the lateral support

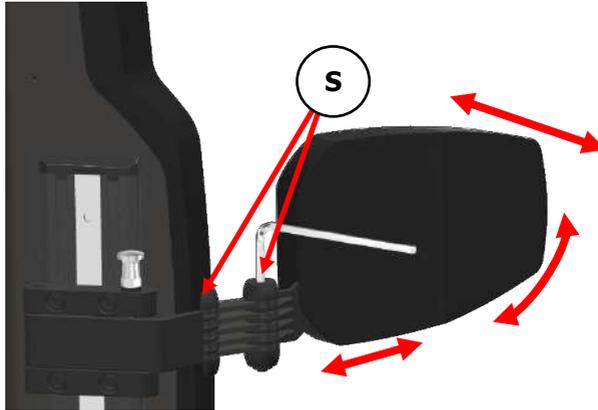


Step 1: Loosen the 2 bolts (**S**) of the friction joints.

Step 2: Move the pad into the required angle, depth and width.

Step 3: Tighten the bolts to fixate the setting.

10.3 Pelvic positioning belt

The optional pelvic positioning belt can be adjusted in length and anchoring point. To change the setting, simply follow the next steps:

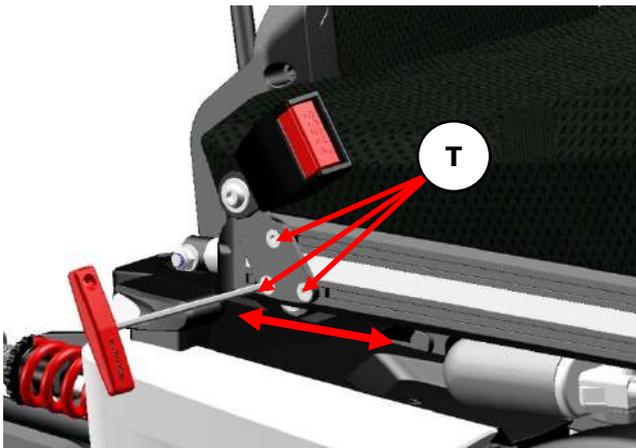

Step 1: Loosen the 3 bolts (**T**) using a 4 mm Allen key.

Step 2: Move the bracket in the required position.

Step 3: Fasten the bolts.



CAUTION

Make sure the brackets are tightened properly to avoid sliding of the seat belt along the seat rail. A sliding seat belt might result in poor seating position of the user.



NOTE


The positioning belt is not to be used as a safety belt. If the wheelchair is transported in an occupied position, the user needs to wear a safety belt which is mounted in the vehicle he or she is transported in.

10.4 Control settings

The side control joystick module is adjustable in depth, height and angle. To set the depth take the following steps:

10.4.1 Height adjustment side control:

To set the height adjustment of the side control follow the next steps:

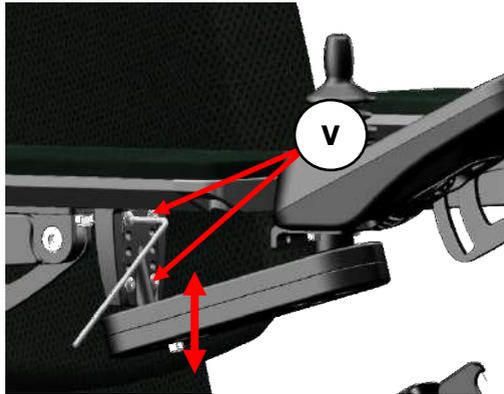


Step 1: Loosen the 4 bolts (**V**) using a 3 mm Allen key.

Step 2: Move the bracket into the required height position.

Step 3: Fasten the bolts again.

10.4.2 Depth adjustment side control

To set the depth adjustment of the side control follow the next steps:

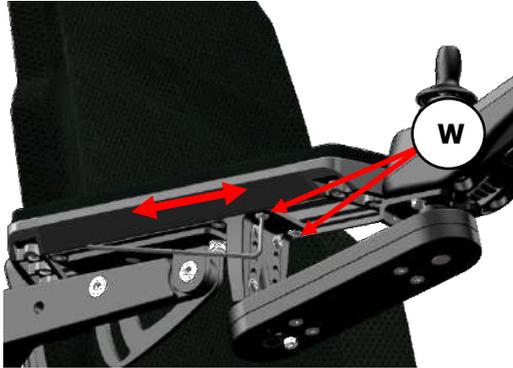


Step 1: Loosen the 2 bolts (**W**) using a 3 mm Allen key.

Step 2: Move the control in the required depth position.

Step 3: Tighten the bolts again.

11. Control panel

The wheelchair uses a color screen joystick module. With this joystick module all functions of the wheelchair can be controlled. This joystick module can be mounted on the left or right armrest or even as an integrated desktop unit.

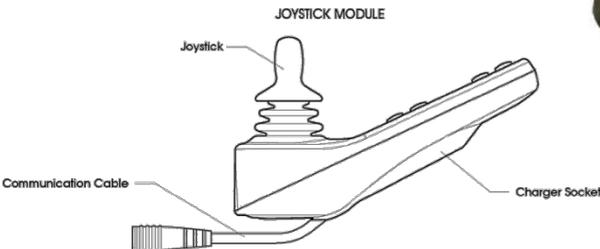

The joystick module contains a few major components which will be explained separately.


11.1 Charging socket

The charging socket is used to charge the batteries. Whilst charging the batteries, the wheelchair driving is automatically blocked.


11.2 Joystick

The primary function of the joystick is to control the speed and direction of the wheelchair. The further you push the joystick from the center position the faster the wheelchair will move. When you release the joystick the brakes are automatically applied. If the wheelchair is fitted with powered seat functions, the joystick can also be used to move and select the specific powered seat function.

Several different shapes of joystick knobs are available to optimize the control of the joystick.

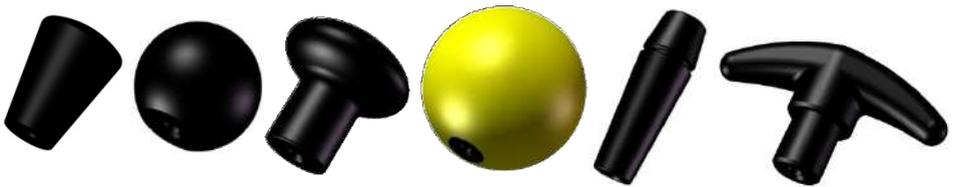

11.3 Display

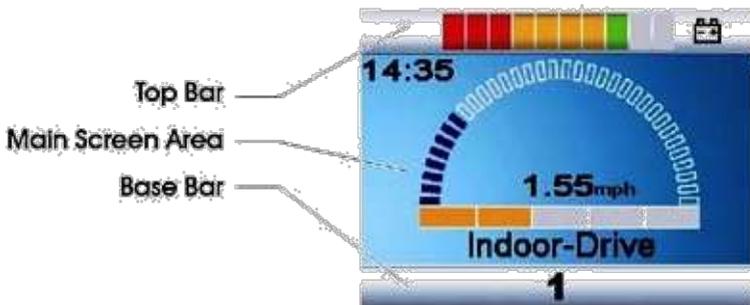

The color LCD screen is split into 3 areas of information: The Top Bar, the Base Bar and the Main Screen Area.

11.3.1 Battery indicator (top bar)



This displays the charge available in the battery and can be used to alert the user to the status of the battery. If all LEDs are on, the batteries are fully charged. If the capacity is lowered one by one an LED will erase. The bar is divided into three color zones: Green, orange and red. If only the LED are left it means the batteries will be almost empty and need to be charged.

Beside the color you also have different LED lighting modes:

LED's Steady: This indicates that all is well.

LED's Flashing Slowly: The control system is functioning correctly, but you should charge the battery as soon as possible.

LED's Stepping Up: The wheelchair batteries are being charged. You will not be able to drive the wheelchair until the charger is disconnected and you have switched the control system off and on again.

11.3.2 Focus light (top bar)



When the wheelchair system contains more than one method of direct control, such as a secondary Joystick Module or a Dual Attendant Module, then the Module that has control of the wheelchair will display the In Focus symbol.

11.3.3 Profile name (main screen)

The profile name shows in which drive profile you are at the moment. The name of the profile can be programmed to your wishes by your local supplier. The wheelchair can have up to 8 different driving profiles. Each profile is set to a certain environment you want to drive in. Standard the wheelchair comes with an indoor- and outdoor profile.



11.3.4 Clock (main screen)

The clock displays the current time in a numeric format. The clock is user adjustable. Adjustable options are:

- Visibility, whether the clock is displayed on screen.
- The display format, 12 or 24 hours.
- The time, the user can adjust the time.




11.3.5 Speed display (main screen)

This gives a proportional display of the wheelchair speed. The Arc begins at 0% and has a programmable maximum. The programmable parameter is Max Displayed Speed. The speeds can be set in mph or km/h. The standard setting km/h.



11.3.6 Speed bar (main screen)


This speed bar displays the current maximum speed setting. It contains 5 steps in speed. These steps can be selected using the speed buttons, explained in the chapter "Buttons"

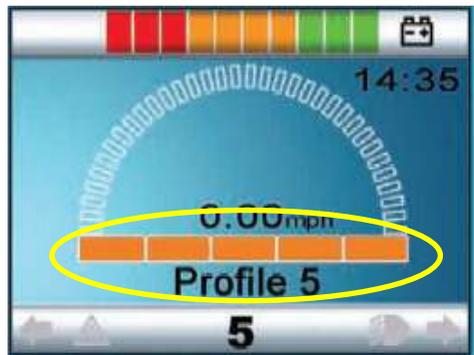

11.3.7 Inhibit (main screen)

If the speed of the wheelchair is being limited; for example, by a raised seat, then this orange symbol will be displayed.

If the driving is stopped by an inhibit, the turtle will flash in red.

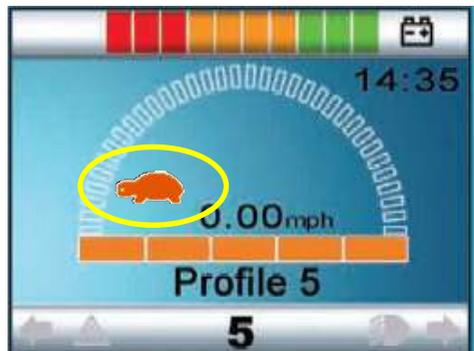

11.3.8 Seat functions (main screen)

Displays the sections of the chair currently selected for movement, the name given to the selection and a direction arrow showing what sort of movement is available.



Besides the screen you use for driving or controlling the seat functions, there are also other screens which show information. The most common screen messages are explained in the next chapters


11.3.9 Additional options (main screen)

Additional screens can show the additional options of the electronic system. For example: Bluetooth, environmental control, mouse function. For more detailed information and about these options, [please contact your local supplier.



11.3.10 Message screen (main screen)

The joystick module displays warning icons and informational messages, in a dedicated message window.

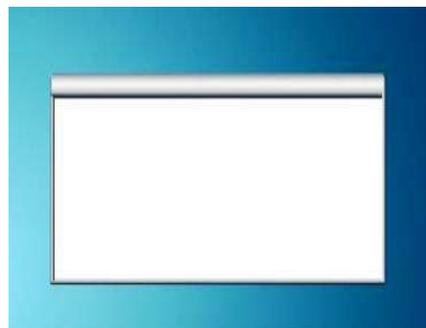

11.3.10.1 Restart message

This icon is shown when the system to be restarted. (Most of the time when a module has been exchanged or added.)



11.3.10.2 Timer message

This symbol is displayed when the control system is changing between different states. An example would be entering Programming Mode. The symbol is animated to show the sands falling.



11.3.10.3 Sleep message

This symbol will be displayed for a short time before the R-net enters into a sleep state.



11.3.10.4 Joystick deflected message

This message is shown if the wheelchair is started up and the joystick is not in its zero position. If you let go of the joystick, the system will start up normally and the message disappears.



11.3.10.5 E-stop message

If the External Profile Switch is activated during drive, or actuator operation, this symbol will be displayed.



11.3.10.6 Error codes

If something is wrong with the wheelchair's electronics, the wheelchair will stop driving and a trip code (error code) will be displayed on the screen of the Joystick module.



For more explanation about the trip code, refer to the “Troubleshooting” chapter.

11.3.11 Current profile (base bar)



The currently selected Profile is shown in numeric form.

11.3.12 Motor temperature (base bar)



This symbol is displayed when the control system has intentionally reduced the power to the motors, in order to protect them against heat damage.

11.3.13 Control system temperature (base bar)



This symbol is displayed when the control system has intentionally reduced its own power, in order to protect itself against heat damage.

11.3.14 Wheelchair lock

The wheelchair has the option to secure against unintended use. Therefore, the joystick module can be locked. This way it is protected against unintended use during storage or parking.


Lock options

The control system of the wheelchair can be locked in two ways: By using a button sequence on the keypad, or with a physical key. This key can be ordered as an accessory.

Keypad locking

To lock the wheelchair by using the keypad lock:

- While the wheelchair is switched on, depress and hold the ON/OFF button.
- After 1 second the control system will beep.
- Now release the ON/OFF button.
- Deflect the joystick forwards until the control system beeps.
- Deflect the joystick in reverse until the control system beeps.
- Release the joystick, there will be a long beep.
- The wheelchair is now locked.
- The following screen will be displayed in the control box:

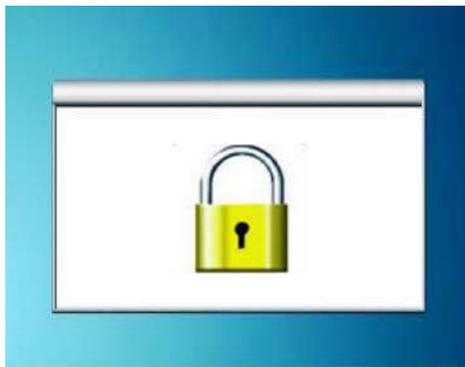

wheelchair in locking mode

To unlock the wheelchair:

- If the control system has been switched off, press the ON/OFF button.
- Deflect the joystick forwards until the control system beeps.
- Deflect the joystick in reverse until the control system beeps.
- Release the joystick, there will be a long beep.
- The wheelchair is now unlocked.

Locking the wheelchair by using a physical key



To lock the wheelchair with the key lock:

- Insert and remove the supplied PGDT key into the charger socket.
- The wheelchair is now locked.

To unlock the wheelchair:

- Insert and remove the supplied PGDT key into the charger socket.
- The wheelchair is now unlocked.

11.4 Buttons

The joystick module has several buttons which will be explained below.



On/Off Button



Speed Buttons
Decrease / Increase



Horn Button



Mode Button



Profile Button



Hazard Button & LED



Lights Button & LED



Left Indicator Button & LED



Right Indicator Button & LED

11.4.1 On/Off button

The On/Off button applies power to the control system electronics, which in turn supply power to the wheelchair's motors. Do not use the On/Off button to stop the wheelchair unless there is an emergency. (If you do, you may shorten the life of the wheelchair drive components).



CAUTION

Always make sure the wheelchair is switched off before entering or leaving the wheelchair. If the wheelchair is switched on during transferring, there is a danger that the joystick will be touched and the wheelchair will move.

11.4.2 Horn button

The horn will sound while this button is depressed.

11.4.3 Speed decrease button

This button decreases the speed setting.

11.4.4 Speed increase button

This button increases the speed setting. (it does not increase the maximum speed!).

11.4.5 Mode button

The Mode button allows the user to navigate through the available operating modes for the control system. The available modes are dependent on programming and the range of auxiliary output devices connected to the control system.

11.4.6 Profile button

The Profile button allows the user to navigate through the available Profiles for the control system. The number of available Profiles is dependent on how the control system is programmed.

Depending on the way the control system has been programmed, a momentary screen may be displayed when the button is pressed.

11.4.7 Hazard Warning Button and LED

This button activates and de-activates the wheelchair's hazard lights. Depress the button to turn the hazards on and depress the button again to turn them off.

When activated the hazard LED and the indicator LEDs will flash in sync with the wheelchair's indicators.

11.4.8 Lights Button and LED

This button activates and de-activates the wheelchair's lights. Depress the button to turn the lights on and depress the button again to turn them off. When activated the lights LED will illuminate.

11.4.9 Left Indicator Button and LED


This button activates and de-activates the wheelchair's left indicator. Depress the button to turn the indicator on and depress the button again to turn it off. When activated the left indicator LED will flash in sync with the wheelchair's indicator(s).

11.4.10 Right Indicator Button and LED

This button activates and de-activates the wheelchair's right indicator. Depress the button to turn the indicator on and depress the button again to turn it off.

When activated the right indicator LED will flash in sync with the wheelchair's indicator(s).

11.5 Jack sockets

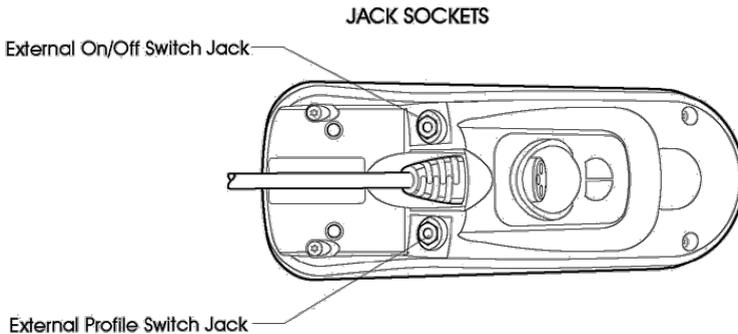

11.5.1 External profile switch jack

This allows the user to select Profiles using an external device, such as a buddy button. To change the Profile whilst driving simply press the button. If the control system is set to latched drive or actuator control operation, then the polarity of the jack input is reversed to affect a failsafe system; meaning this input will provide an External Profile Switch function and an Emergency Stop Switch function.

11.5.2 External on/off switch jack

This allows the user to turn the control system on and off using an external device, such as a buddy button.



NOTE

The Joystick Module is supplied with rubber bungs that must be inserted into the Jack Socket when no external device is connected.

11.6 R-net Connectors


To connect the Communication Cables:

- Holding the connector housing, firmly push the connector into its mate until you can no longer see the yellow plastic.

The connectors are secured using a friction system.

To disconnect the Communication Cables:

- Holding the connector housing firmly, pull the connectors apart.

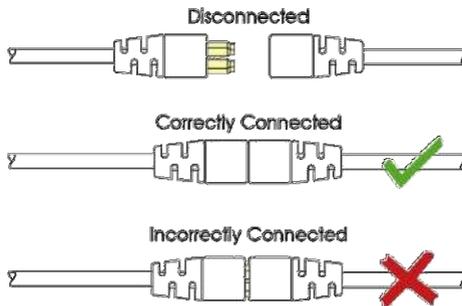

Do not hold or pull on the cable. Always grip the connector when connecting and disconnecting.


When the control system is first switched on after a connection, or system component change, the Timer will be displayed whilst the system checks itself and then the re-start icon will be displayed. Switch the control system off and on again to operate.




CAUTION

If the communication is poor because of damaged cables, a trip code "bad cable" might be shown on the display. Should this message appear on the display contact your local supplier to have the wheelchair checked.

11.7 Joystick

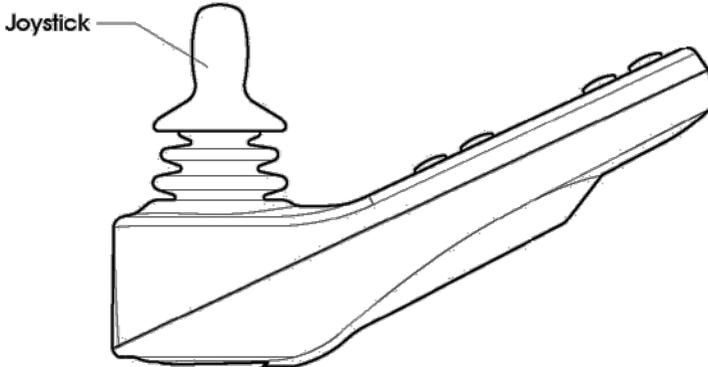

The joystick is primarily used to drive the wheelchair. just push the joystick into the direction you want to drive, and the wheelchair will start to move in that direction.

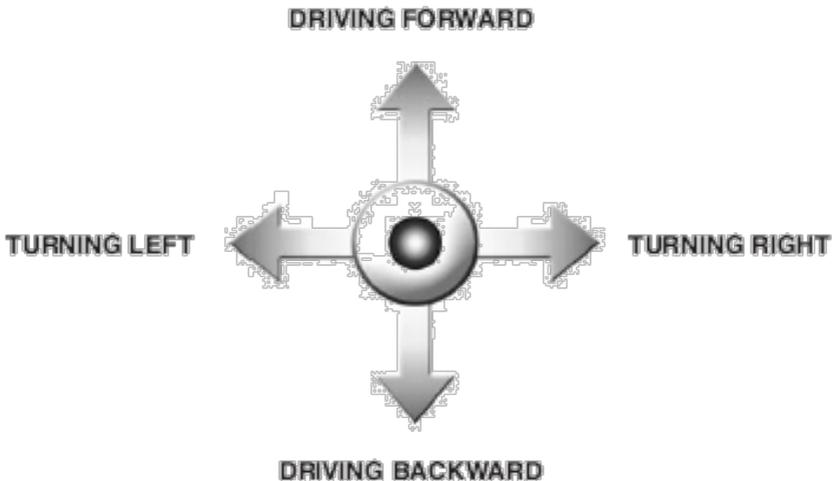

The secondary purpose of the joystick is to navigate through main menu of the wheelchair. By moving the joystick forward or backward you can scroll up or down through the menu; by moving to the right, you can enter a sub selection.



CAUTION

We strongly recommend practicing the function of the joystick before starting to drive with the wheelchair.

12. Electric system

12.1 Batteries

The wheelchair has two serial connected 12-volt maintenance-free batteries for the power supply. The capacity of the batteries can be 60, 72 or 85 Amps. The batteries are fitted in the center of the chassis to arrange a low center point of gravity. Both batteries are easy accessible for maintenance or replacement.



Position and access of the maintenance-free batteries



CAUTION

- Be careful when using metal objects close to the batteries. A short circuit might easily create strong sparks and can cause a fire. Should you need to work on the batteries, use isolated tools and wear protective gear on hands and eyes.
- Batteries are chemical components and shall be treated as such. In case of removal, one shall treat the batteries as chemical waste. The batteries need to be disposed according to the local regulations for chemical waste.

12.2 Fuses

The wheelchair has one main fuse to protect the batteries against overload and short circuit. This main fuse is placed between the rear casters and easy accessible. The electronics itself is completely protected against short circuit and overload.



Position of the main fuse

The main fuse is also used to disconnect the batteries from the electronics. This is required when transporting the wheelchair on a plane.

Additional fuses

Beside this main fuse there is a fuse on each battery close to one of the connecting pole. They are integrated into the battery cable. This is to protect each battery separate for short circuit. These fuses are stronger than the main fuse, so in case of a short circuit, the main fuse will blow first.



CAUTION

- If the fuse is blown, please contact your local authorized supplier. He should check the wheelchair first before replacing the main fuse. The fuse only blows if a serious problem occurs.
- Only use original spare part fuses of KARMA. Using other fuses might damage the electronic system or even cause fire.

13. Using the wheelchair

13.1 General warnings and advices

Please read this section of the manual very carefully as it contains issues related to safety and possible hazards.



WARNING

- When the user is driving the wheelchair for the first time, the supplier has to make sure that the maximum driving speed and curving speed are set in a slow mode. After learning to drive the wheelchair safely, the set speeds can be increased.
- Special care should be taken in driving on unequal surfaces such as slopes, unequal pavements and during descending from footpaths.
- It is not allowed to carry passengers other than the user on the wheelchair.
- On slippery surfaces, like ice and snow, the driving speed must be reduced accordingly.
- Do not drive through water puddles, you cannot see how deep they are. This might lead to dangerous situations. Water can damage the wheelchair.
- Only charge the wheelchair in well-ventilated areas.
- Note that no other persons or animals are in the direct contact zone of the wheelchair when using it. This is for both driving and using the high low. Because the wheelchair is a very powerful machine with a relative high weight this might lead to severe injuries.
- When driving the wheelchair in the dark, be sure that you have the lights switched on.
- Always drive slowly in the near surroundings of other people or animals.
- Although the wheelchair is intensively tested, it cannot be excluded completely that the wheelchair influences the performance of electromagnetic fields (e.g. Alarm systems of shops, automatic doors etc.).
- The driving characteristics of the wheelchair can be influenced by strong electromagnetic fields (e.g. Those emitted by portable telephones, electricity generators or high-power sources. Try to avoid the near presence of any radiation source such as radio's, cell phones etc. If your



WARNING

wheelchair reacts to a source of radiation with unexpected behavior, try to drive slowly to a safe place, turn off your wheelchair and try to extinguish the radiation source.

13.2 Use in combination with other products

Different- or customized seat:



WARNING

- The combination of seat and user does not exceed the maximum allowed weight on the wheelchair carrier and tilt mechanism (136 kg).
- The seat is fixed properly to the seat post.
- The center of gravity of the combination of user and seat is on the same spot as when the standard seat would be used.
- The position of the tray table and/or the control unit is comfortable and easy to use for the user.
- The used materials are in compliance with the accepted standards mentioned in EN 12184 regarding flame resistance and bio-compatibility.
- The seat or any other mounted parts do not touch the wheelchair carrier when using the high low function. This is because the dimensions will vary from the standard seat. This has to be checked by watching these parts when activating the high low.
- The seat or any other mounted parts do not touch the wheelchair carrier when using the tilt function. This is because the dimensions will vary from the standard seat. This has to be checked by watching these parts when tilting the chair.
- Changes which are made by third parties are not covered by the warranty and responsibility of KARMA Medical.

13.3 Hot and cold surfaces



WARNING

- Some parts of the wheelchair can reach high temperatures when exposed to direct sun. Please be careful with touching especially the plastic parts under these circumstances in order to prevent skin burning.
- The wheelchair can reach low temperatures when exposed to cold weather (below zero degrees Celsius). Please take caution in touching especially the metal parts with wet body parts under these circumstances as they easily can freeze and get stuck to these surfaces.

13.4 Danger of pinching

User

Special care has been taken to make sure that the chance that the user pinches him or herself while seated in the wheelchair is minimal. However there are few situations that might lead to injury. Special caution has to be taken under the following circumstances:

- When the tray table is closed, pinching of fingers or other body parts is possible between the locking parts.
- When the revolving control unit is used in the tray table, pinching of fingers or other body parts is possible when the control unit is being turned upside down.
- When adjusting the seat while the user is sitting in the chair, please note that no body parts are in the direct zone of the moving parts.



WARNING

- When moving the seat down, the tilt frame comes very close to the top chassis cover. This creates a pinching danger, when at this time, hands are on the top cover at the rear end of the chassis. For this reason, a warning decal is placed on the top cover on the rear of the chassis. We advise you to always keep your hands or the hands from other



WARNING

persons away from the rear end of the top chassis cover.

- All areas where there might be a risk of pinching are indicated by this warning decal:



13.5 Surroundings

Special care has been taken to make sure that the chance that the surroundings pinch him or herself is minimal. However there are few situations that might lead to injury. Special caution has to be taken under the following circumstances:

- When driving the wheelchair, make sure that no persons or animals are in the near surroundings, because running over e.g. feet will lead to serious injury as a result of the high weight of the electrical wheelchair.
- When using the seat lift and/or the electrical tilt adjustment, make sure that no persons or animals are in the near surroundings, because it is possible to get pinched by the moving mechanism, although the moving parts are designed to be as safe as possible.

13.6 Precautions to prevent dangerous situations

In order to prevent dangerous situations please take note of the following precautions:

- Only charge the battery in well-ventilated areas.
- Only drive at slow speed in the direct surrounding of other people or animals.
- Always turn on the front and rear lights when using the chair under circumstances with limited sight like darkness or fog.

- Please do not allow any people to stand or sit in the wheelchair, except for the user.
- Make sure that the remaining battery power is sufficient for the distance that is to be bridged.
- Do not replace a damaged fuse before it is known why the fuse is blown and the cause is taken away.
- Have the wheelchair checked by your supplier after any collision or when the wheelchair is otherwise (visual) damaged.
- Check the tire pressure and refill the tires if necessary every four weeks. Check the tires at the same time for wear and damage. Replace them if necessary.
- Have the wheelchair checked on a yearly basis by your supplier.
- Do not change the programmed driving characteristics of your control unit, as it is specific for the situation of the user. If any adjustment is required because of a change of circumstances, please contact your supplier.



WARNING

Always make sure that, when positioned on slopes, the brakes are engaged (no Freewheel).

If the wheelchair is in freewheel mode, there is a risk that the wheelchair might start to move in an uncontrolled way. This might lead to personal or material damage.

13.7 Use on slopes: driving on downhill slopes

Driving on downhill slopes must always be done at a low speed and with great care. Avoid sudden braking, abrupt avoidance maneuvers and never maintain a speed higher than that at which you can maneuver the wheelchair in a safe and secure manner. Always be aware of the fact that the control of the wheelchair driving downhill is different than on level surfaces.



NOTE

- When driving on downhill slopes with an uneven or slippery surface (for example grass, gravel, sand, ice or snow) you should drive with extra care and attention.
- When driving on downhill you can use the tilt (if built in) to create a more stable seating position for yourself.



WARNING

- Never drive downhill on slopes larger than 10°. This might result into uncontrollable behavior of the wheelchair. This can lead to material or personal damage (Dynamic stability according to ISO 7176-2= 6°).
- The position of the seat in height and angle or the position of the backrest has great influence on the stability of the wheelchair when driving on slopes. Make sure the seat is in the optimal driving position to avoid tipping over.
- The position of the seat in height and angle or the position of the backrest has great influence on the stability of the wheelchair if driving on slopes. Make sure the seat is in the optimal driving position to avoid tipping over.

13.8 Use on slopes: driving on uphill slopes

Driving on uphill slopes must always be performed with great care and attention. Avoid sudden avoidance maneuvers and never drive at a speed higher than needed to maneuver the wheelchair in a safe and secure way. Avoid holes and bumps as much as possible. Drive slowly and controlled.



NOTE

- When driving on uphill slopes with an uneven or slippery surface (for example grass, gravel, sand, ice or snow) you should drive with extra care and attention.
- When driving on uphill you can use the tilt (if build in) to create a more stable seating position for yourself.




WARNING

- Never drive uphill on slopes larger than 10°. This might result into uncontrollable behavior of the wheelchair. This can lead to material or personal damage (Dynamic stability according to ISO 7176-2= 6°).
- The position of the seat in height and angle or the position of the backrest has great influence on the stability of the wheelchair if driving on slopes. Make sure the seat is in the optimal driving position to avoid tipping over.

13.9 Driving on sideways slopes

Driving on a sideways slope must always be performed with great care. Avoid sudden avoidance maneuvers and never drive at a speed higher than needed to maneuver the wheelchair in a safe and secure way. Avoid holes and bumps as much as possible. Drive slowly and controlled.

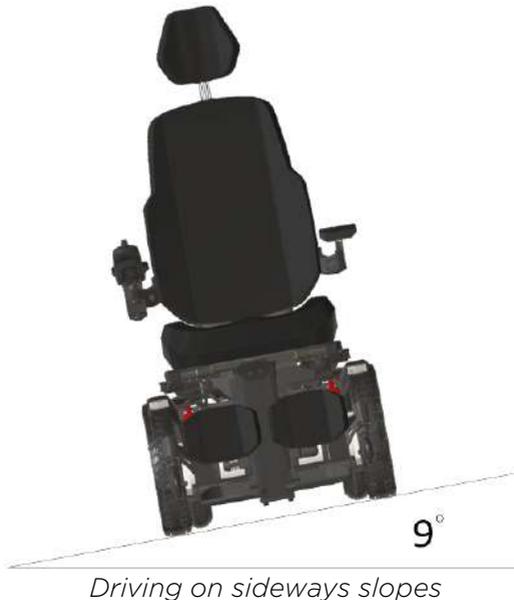



NOTE

When driving on sideways slopes with an uneven or slippery surface (for example grass, gravel, sand, ice or snow) you should drive with extra care and attention.



WARNING

- Never drive sideways slopes larger than 9°. This might result into uncontrollable behavior of the wheelchair. This can lead to material or personal damage (Dynamic stability according to ISO 7176-2= 6°).
- The position of the seat in height or the position of the backrest has great influence on the stability of the wheelchair if driving on slopes. Make sure the seat is in the optimal driving position to avoid tipping over.

13.10 Obstacle climbing

Do not drive the wheelchair over obstacles of a height larger than 70 mm. driving over tall edges increases the risk of tipping over as well as the risk of damage to the wheelchair. Always be aware when climbing obstacles of the stability of your wheelchair.



Driving down of a higher surface (like pavement), Always be aware of the sudden forward movement of your wheelchair when driving down of it. If your wheelchair has powered seat tilt, you can use the seat tilt for more stability whilst driving of the pavement.



NOTE

When driving over obstacles with uneven or slippery surface (for example grass, gravel, sand, ice or snow) you should drive with extra care and attention.



WARNING

Never drive on obstacles higher than 70 mm. Always drive with maximum attention and great care.

13.11 Use in presence of electromagnetic fields, e.g. from cell phones

Use your cell phone only when the wheelchair is switched off. Although the wheelchair is tested and approved for electromagnetic interference, there is a very small chance that strong electromagnetic fields from cell phones or some other electrical products lead to unexpected and unpredictable electrical reactions from the wheelchair.

Try to avoid the near presence of any radiation source such as radio's, cell phones etc. If your wheelchair reacts to a source of radiation with unexpected

behavior, try to drive slowly to a safe place, turn off your wheelchair and try to extinguish the radiation source.

When it is unavoidable to use the wheelchair under these circumstances, be prepared for any unexpected and unpredictable electrical reactions from the wheelchair.



WARNING

- If you enter an area where there might be a risk of strong electromagnetic interference, always reduce your driving speed and drive carefully.
- Avoid area's closeness where strong military transmitters are used. They might interfere with your wheelchair's electronics.
- Avoid area's closeness to high voltage power lines. They might interfere with your wheelchair's electronics.
- Avoid area's closeness to high frequency energy equipment, like high frequency welding machines. They might interfere with your wheelchair's electronics.

14. Driving the wheelchair

The wheelchair is designed for indoor and outdoor use. When driving indoors, you must be careful when driving in, for example, narrow passageways, when passing through doors and entryways as well as when using elevators, ramps, etc. Also be aware of the risk of things getting caught in the machinery when you use the electrical seat lift and seat tilt, in particular when the wheelchair has been run in under a table, workbench or something like that.



WARNING

Always make sure the wheelchair is switched off before entering or leaving the wheelchair. If the wheelchair is switched on during transferring, there is a danger that the joystick will be touched and the wheelchair will move.

Outdoors, you must remember to drive very slowly on steep downhill slopes and to be very careful when driving on uneven surfaces, on uphill slopes, with sideways slopes and when negotiating obstacles. Always maintain a safe distance from the edge when driving close to drop-offs and pavements.



NOTE

We recommend that you should make repeated test drives in areas in which you know you feel secure so that you are quite familiar with how the wheelchair and its accessories behave in different situations before you begin using the wheelchair on normal roads and other public areas.

14.1 Driving in general

Make sure that the control system is mounted right and that the joystick position is correct. The hand or limb you use to operate the joystick should be supported, for example by the wheelchair armrest. Do not use the joystick as the sole support for your hand or limb, the wheelchair movements and bumps could upset your control, which might result in uncontrolled driving.

1. Switch on the power by pressing the on/off button on the control panel.

2. Select the right profile (start with the indoor profile).



WARNING

Always make sure the wheelchair is switched off before entering or leaving the wheelchair. If the wheelchair is switched on during transferring, there is a danger that the joystick will be touched, and the wheelchair will move.

3. Set an appropriate maximum speed by pressing the decrease or increase button until the desired indicator lamp lights up for your type of driving. It is preferable to begin with a low speed.
4. Carefully move the joystick forward to drive forward, and backward to drive backward.
5. The speed of the wheelchair is adjusted continuously by the joystick being moved different distances forward and backward respectively. The wheelchair's electronics make creep driving possible over edges (max. 70 mm). You can drive up to the edge, and then carefully drive over it.

When you drive through the long and steep slopes, to keep the motors from overheating, the chair could be in protective mode. When the chair is in this mode, it will slow down automatically and a red flashing symbol will appear on the screen of the joystick module.

When it happens, you need to move to a safe area immediately. Then wait for 150 seconds until the system is restoring itself and the red flashing symbol disappears.



WARNING

- Before the red flashing symbol disappears, operate the joystick cautiously to prevent the chair from sliding down on the slopes.
- Do not perform the first test drive on your own. The test drive is of course just a check of how you and the wheelchair function together, and




WARNING

you may need some assistance.

Before driving, check that the wheel freewheel is set in the drive position.

14.2 Driving technique

The electronic control system of the wheelchair “reads” your joystick movements and transforms these “commands” into movements of the wheelchair. You will need very little concentration to control the wheelchair, which is especially useful if you are inexperienced. One popular technique is to simply point the joystick in the direction you want to go. The wheelchair will move in the direction you push the joystick. Always think about driving as flexibly and fluently as possible and avoid heavy braking and avoidance maneuvers. The smoother you move the joystick, the smoother the wheelchair will

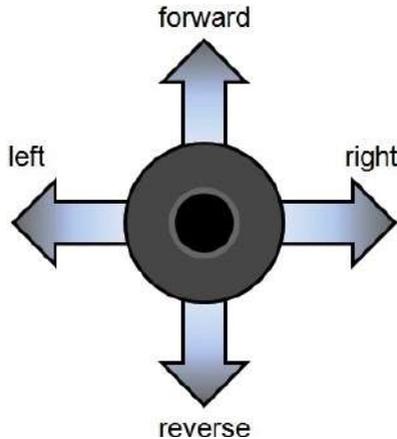

14.3 Stopping the wheelchair

If you would like to stop, simply move the joystick slowly towards the center and release the joystick. The wheelchair will come to a gentle stop. If you want to stop more quickly, simply let go of the joystick. It will put itself back into neutral position, which makes the wheelchair stop. Is there an emergency

and you need to make an emergency stop, pull the joystick backwards. This will slow down and stop the wheelchair very fast.



WARNING

- Be careful driving backwards. You cannot really oversee where you are driving. It is better, when the space is available, to turn around and drive forward. By driving backwards not seeing where you are heading you might bump into something or someone. This can lead to personal or material damage.
- Be careful using the emergency brake. Especially when driving on slopes. Extreme braking might create the risk of tipping over when you are on a slope. Also, be aware that during braking you tend to lose balance yourself. If not strapped into a seat belt you might run the risk of falling out of your wheelchair whilst braking very hard.

15. Using the powered seat functions

If your wheelchair has powered seat functions like seat lift, seat tilt, backrest recline and/or powered legrest, you can control them by using the menu on the joystick module.



15.1 Seat lift

To enter the seat lift function menu, push the button "Mode" on the joystick module. You will leave the drive mode and get into the seat function mode.



Seat lift screen in the menu

By moving the joystick to the left or right you can switch between different powered seat functions. if you want to move the seat lift, move the joystick side ways until you see the seat function "Lift". Now move the joystick backwards and the seat lift will start to move upwards. As long as you pull the joystick backwards, the seat lift will move up. Release the joystick and the seat lift movement will stop. Push the joystick forward and the seat will tilt into forward position.




NOTE

- The acceleration and speed of each seat function can be programmed by your local authorized supplier. Should you request a different setting, please contact your local authorized supplier.
- The default movement of deflection is set to backwards for lifting the seat up. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.2 Seat tilt

To enter the seat tilt function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and getting into the seat function mode.

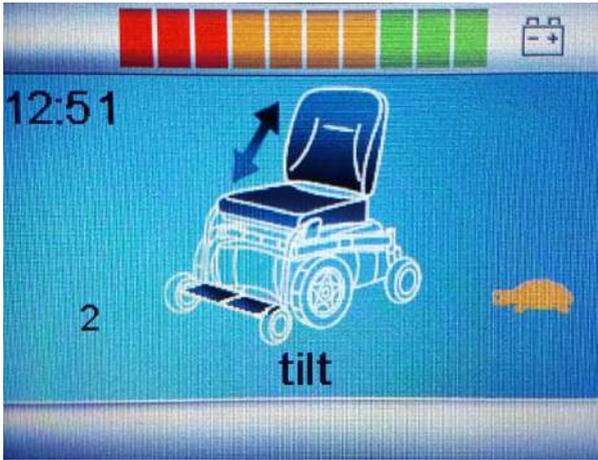

Seat tilt screen in the menu

By moving the joystick to the left or right you can switch between different powered seat functions. if you want to move the seat tilt, move the joystick side ways until you see the seat function "tilt". Now move the joystick backwards and the seat tilt will start to tilt backwards. As long as you pull the joystick backwards, the seat tilt will tilt backwards. Release the joystick and the seat tilt movement will stop. Push the joystick forward and the seat will tilt into forward position.




NOTE

- The acceleration and speed of each seat function can be programmed by your local authorized supplier. Should you request a different setting, please contact your local authorized supplier.
- The default movement of deflection is set to backwards for tilting the seat backwards. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.3 Backrest

To enter the backrest recline function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and getting into the seat function mode.

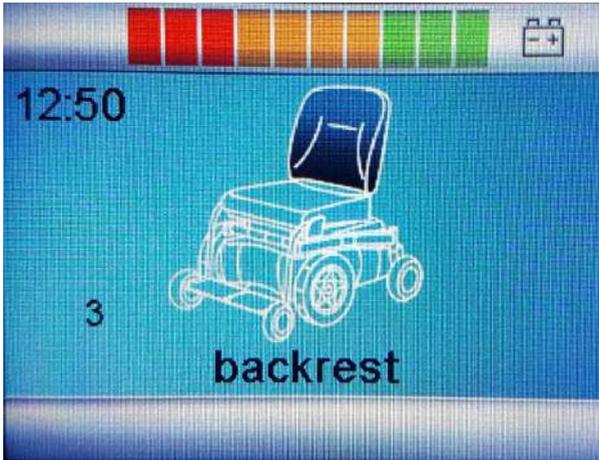

Backrest recline screen in the menu

By moving the joystick to the left or right you can switch between different powered seat functions. if you want to move the backrest function, move the joystick sideways until you see the seat function "backrest". Now move the joystick backwards and the backrest will start to recline backwards. As long as you pull the joystick backwards, the backrest will recline backwards. Release the joystick and the backrest movement will stop. Push the joystick forward and the backrest will recline into forward position.



NOTE

- The acceleration and speed of each seat function can be programmed by your local authorized supplier. Should you request a different setting, please contact your local authorized supplier.
- The default movement of deflection is set to backwards for reclining the backrest backwards. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.4 Legrest

To enter the legrest adjustment function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and getting into the seat function mode.



Backrest recline screen in the menu

By moving the joystick to the left or right you can switch between different powered seat functions. If you want to move the legrest function, move the joystick sideways until you see the seat function "legrest". Now move the joystick backwards and the legrest will start to stretch and go up. As long as you pull the joystick backwards, the legrest will go up into stretch. Release the joystick and the legrest movement will stop. Push the joystick forward and the legrest will lower itself into a lower position.



NOTE

- The acceleration and speed of each seat function can be programmed by your local authorized supplier. Should you request a different setting, please contact your local authorized supplier.
- The default movement of deflection is set to backwards for stretching the legrest. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.5 Support wheels

To enter the support wheels adjustment function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and getting into the seat function mode.



Support wheels screen in the menu

Move the joystick to the left or right until you see the seat function "support wheels". Now move the joystick backwards and the support wheels will move up. As long as you pull the joystick backwards, the support wheels will lift up. Release the joystick and the support wheels movement will stop. Push the joystick forward and the support wheels will move down.



WARNING

- The support wheels also work as anti-tippers. For that reason, the support wheels are placed around 50 mm above the ground. In this position it is possible to drive at maximum speed. If the wheels are in a lower or higher position, the driving speed is automatically reduced.
- If you want to use a ramp to drive into a building or vehicle, make sure you first raise the support wheels to ensure the drive wheels of the wheelchair keep traction. Do not forget to put the supports wheels back into the normal drive position again to be able to drive at maximum driving speed.

15.6 Relax position

To enter the support wheels adjustment function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and getting into the seat function mode.



Relax position screen in the menu

Move the joystick to the left or right until you see the seat function "relax". Now move the joystick backwards and the seat will go in to the relax (laying) position. As long as you pull the joystick backwards, the seat will stretch itself. Release the joystick and the movement will stop. Push the joystick forward and the seat will get back in to the seating position again.




NOTE

- The acceleration and speed of each seat function can be programmed by your local authorized supplier. Should you request a different setting, please contact your local authorized supplier.
- The default movement of deflection is set to backwards for relaxing the seat backwards. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.7 Negative tilt

To enter the support wheels adjustment function in the menu, push the button "Mode" on the joystick module. You will leave the drive mode and get into the seat function mode.

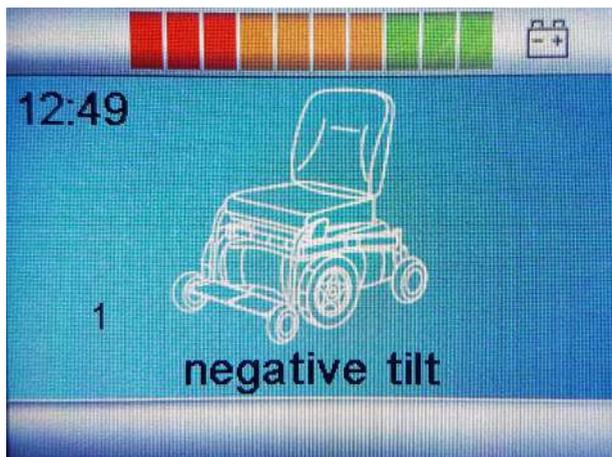

Relax position screen in the menu

Move the joystick to the left or right until you see the seat function "negative tilt". Now move the joystick forward and the seat will tilt into the forward direction. As long as you pull the joystick forward, the seat will tilt forward. Release the joystick and the movement will stop. Push the joystick backwards and the negative seat tilt will get back in to the seating position again.



NOTE


- The negative tilt can only be used if first, the legrest is stretched to 45 degrees angle. This is to avoid a collision with the chassis when tilting forward.
- The default movement of deflection is set to forward for tilting forward. Should you want to switch the axis direction of the joystick, please contact your authorized dealer to have the deflection set in the opposite direction.

15.8 PRO-Motion function

Pro-Motion is a function for different purposes:

1. Stretch/reach out function, being able to reach out to grab things from shelves or handing over money to the person behind a counter.
2. To transfer in- or out of the wheelchair by raising the seat height and tilting the seat to a negative seat angle. This way it is easier for a user to exit the wheelchair, with the help of a care giver/attendant person.

The setting of the end position of the Pro-Motion function can be individually adjusted/programmed and stored by the dealer, to fit the specific user request. The negative seat pan angle can be set up to 45°. The seat height, backrest angle and legrest can also be set to fit the requirements of the user.

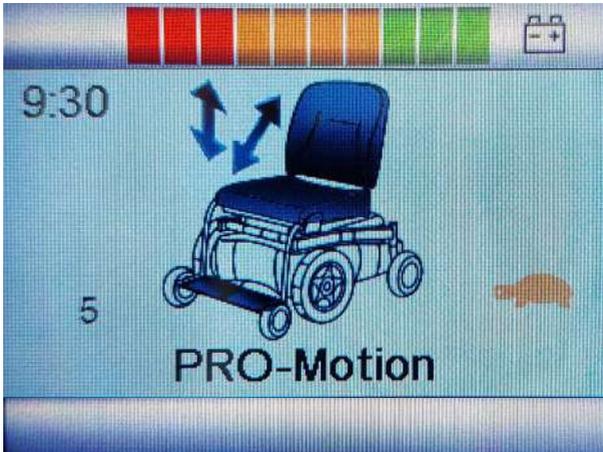

PRO-Motion position screen in the menu



NOTE

- When using the PRO-Motion function, we suggest adding the additional knee support to ensure stability during the PRO-Motion movement. If there are any upper body instabilities, a chest belt might be suitable as well.
- When using the PRO-Motion function to have a better reach, the driving speed will be reduced to very slow.
- If the PRO-Motion function is used for transferring in or out of the wheelchair, the seat height can be in a way that the footplates are flat on the ground. This makes transferring out or into the wheelchair safe and easier. In that situation the driving will be blocked to avoid scratching the floor or sudden movements of the wheelchair by accidentally touching the joystick.
- Seat height, seat angle, backrest angle and legrest angle can be individually set to the users' requirements.

15.9 Using additional function of the wheelchair menu

If your wheelchair has additional function build in like the Bluetooth mouse function, you are able to control this using the menu and joystick.

To enter the Bluetooth mouse menu, push the button "Mode" on the joystick module. You will leave the driving mode. The first screen you will see is the powered seat function screen. If you push the "mode" button once more, you will enter the Bluetooth screen. Now the joystick becomes the mouse for using the PC or laptop.

For further information about the additional options, we refer to your local authorized supplier.




16. Handling the mechanical brakes

The drive motors of the wheelchair have electromechanical brakes. The brake can be released to set the wheelchair into freewheel mode. In freewheel mode the wheelchair can be pushed. This might be necessary to move the wheelchair in certain cases.

16.1 Release the mechanical brakes

To release the mechanical brakes, take the following steps.

Look for the red lever on each of the driving motor. Around the lever is a instruction sticker which shows the direction to open or lock the mechanical brake. Move the lever into the "open" position on each motor. Now the wheelchair is in freewheel mode and can be pushed.

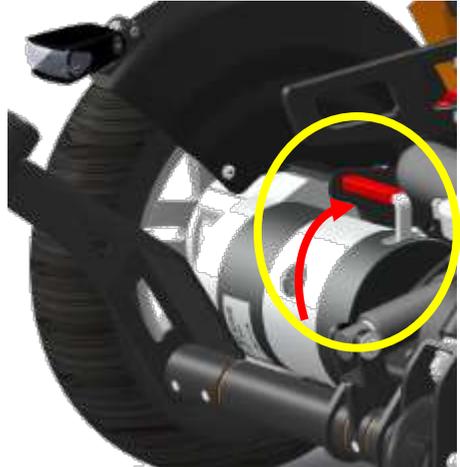

To lock the brakes, move the lever in to the "lock" position. on both motors.



NOTE

If you want to put the wheelchair into freewheel mode, be sure to switch the electronics first. Leaving the electronics switched on will result in a large resistance whilst pushing in freewheel mode.



WARNING

- If the parking brake is released (free-wheel mode), the wheelchair cannot be driven by the electronics. Therefore, the release of the brakes should only be done in emergency cases and or for servicing. If the user is on board, the parking brakes should always be attached.
- Always make sure that, when positioned on slopes, the brakes are engaged (no Freewheel). If the wheelchair is in freewheel mode, there is



WARNING

a risk that the wheelchair might start to move in an uncontrolled way. This might lead to personal or material damage.

17. Charging the maintenance-free batteries

The amount of charge in your maintenance-free batteries depends on a number of factors, including the way you use your wheelchair, the temperature of the maintenance-free batteries, their age and the type of maintenance-free batteries used. These factors will affect the distance you can travel in your wheelchair. All wheelchair maintenance-free batteries will gradually lose their capacity when they get older. The most important factor that is reducing the life span of your batteries is the amount of charge you take from the batteries before you recharge them. The maintenance-free battery life is also reduced by the number of times you charge and discharge the batteries. Normally the number of cycles is between 300 and 700 times. To make your maintenance-free batteries last longer, do not allow them to become completely discharged. Always recharge your maintenance-free batteries promptly after they are discharged. If your battery gauge reading seems to fall more quickly than usual, your batteries may be worn out. If your wheelchair shows these indications, please contact your local authorized supplier to have the maintenance-free batteries checked.

17.1 Battery level

The power level of the batteries is displayed on the LCD screen of the joystick module.



Battery indicator

If the maintenance-free batteries are fully charged, all ten LEDs on the top bar light up. The more energy is used the more LED extinguish, starting on the right side.

If only the red LED are still on, it indicates that recharging of the maintenance-free batteries is required.

If only two red LEDs are flashing, it indicates that the maintenance-free batteries are empty and should be charged immediately.



NOTE

- If the battery indicator shows only two segments in flashing, you should charge the batteries as soon as possible. This flashing is a warning signal. You are still able to drive the wheelchair but only for a short distance. If the batteries reach a level where they cannot supply enough energy to control the wheelchair in a safe way. The wheelchair will stop and give an error warning saying "low battery voltage".
- If the batteries should be drained completely, it is important that you charge them up again as soon as possible since a complete loss of charge reduces the lifespan of the batteries.
- Information about the charger which is supplied with the wheelchair can be found in the user manual of the charger itself. You can find the charger user manual in the tool bag which comes with the wheelchair.
- Some local dealers supply the wheelchair with their own brand of batteries and battery charger. For information about these batteries and charger, you should ask your local authorized supplier.

17.2 Charging socket

The charger socket can be found on the front side of the joystick module. If the wheelchair has an integrated desktop control, the charger socket will be on the side of the joystick module.



Charger socket position



Battery charger

The wheelchair can be delivered with a battery charger. This charger has a capacity to charge up to 11 amperes. This charger will fully charge the batteries within 8 hours.



NOTE

- For more detailed information about the charger and its functions, we refer to the manual which comes with the charger.
- In some occasions putting in the charger socket yourself can be very difficult. Sometimes you would like to have the charger socket on a specific place on your wheelchair. For this reason, the wheelchair has an additional charger socket which can be placed on the spot you can reach yourself. For more information, please contact your local authorized supplier.
- Be sure that the charger plug is pushed fully in position. You will not be able to drive the wheelchair when the charger is connected. If the wheelchair does drive with the charger plugged in, contact your local authorized supplier.
- In some occasions it might be the case that your local supplier will deliver the wheelchair with a different brand charger. In that case your local supplier will inform you about the functionality of that charger and will also make sure the charger comes with a user manual.

17.3 Disposal of broken or worn-out batteries



Batteries don't last forever. Therefore, batteries need to be changed after a certain period. The safest way is to have this done by authorized personnel of your local supplier. Batteries are chemical waste and need to be treated as such, using protective clothing, gloves and glasses.




WARNING

- Replacing damaged or old batteries needs to be done by authorized personnel wearing protective clothing, gloves and safety glasses.
- Old or damaged batteries are classified as chemical waste and need to be disposed according to the local regulations for chemical waste. Please contact your local supplier for further details.

18. Transport of the wheelchair

18.1 4-point tie down restraint system

The wheelchair must only be transported in a vehicle that is approved or adapted for such purposes. It is safest if the wheelchair is separated from the driver's compartment. Transportation in a trailer is also an optional recommendation. Should the wheelchair be transported in an MPV/estate car or other vehicle, it is vital that the wheelchair is properly fixed and that the fixing points of the car are well anchored. In all situations of transportation, the wheelchair needs to be properly fixed using a 4-point heavy duty webbing restraint to prevent the wheelchair from sliding or tilting while driving. Check that the wheelchair is properly fastened and that the parking brakes are engaged. The wheelchair can be locked into position by using fastening straps through the brackets in the front and the back, each marked with an indication sticker.

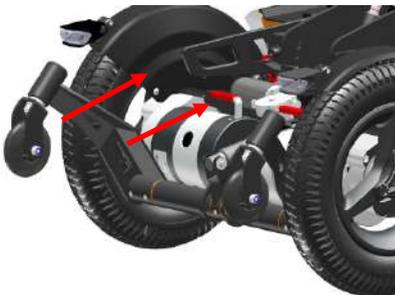

Front tie-down loops



Rear tie-down loops



NOTE

The specifications of the wheelchair are in accordance with the requirements specified in ISO 7176-19 – 2008.

Secure the wheelchair according to the manufacturer of the vehicle restraint systems instructions. Always make sure that the fastening points on the transport vehicle are well anchored. Use of this is strongly advised since the heavy wheelchair can cause serious problems in case of a car accident. The wheelchair fulfils all requirements according to the ISO 7176-19 – 2008 standard (“Wheeled mobility devices for use as seats in motor vehicles”).



NOTE

- KARMA Medical Taiwan would always recommend transferring to a car seat within a vehicle; however should this not be possible, the following is the safest method:
 - a. The wheelchair must be positioned in a forward-facing position.
 - b. An Unwin restraint system like model Gemini 3 or a different brand with equivalent specification must be used.
 - c. As a car safety belt a Klippan Safety AB belt, model 907428 or a different brand with equivalent specification must be used.
 - d. The restraint system must be fixed on the specific points of the wheelchair, which show a label of a transportation hook.
 - e. A head restraint system must be fitted during transportation. This device must be suitably positioned and able to stay on during transportation.
 - f. The centre point of gravity of the wheelchair during transportation should be as low as possible. A powered seat elevator must be in its drive position, the backrest should be upright, the seat should be in a horizontal position and the legrest should be positioned in a normal seating positions.
 - g. During transportation the wheelchair should be switched off to prevent it from moving by accidental joystick use.



NOTE

- h. Make sure the tire pressure of each wheel of the wheelchair is in the optimal condition. Too low tire pressure can result in a instable behavior of the wheelchair during transportation.
- The position belt of a wheelchair is not meant to be used as a car safety belt. It only prevents the user from sliding out of the seat while driving the wheelchair. If a user is transported in his wheelchair, he or she should wear an extra car safety belt, which is attached to the vehicle like all the car safety belts.
- When shipped by boat, please give special attention to prevent contact with saltwater or air. Saltwater is extremely corrosive and might lead to unwanted damage of the product.

18.1.1 Transportation guideline

The wheelchair has a 4-point heavy duty webbing restraint. Using two brackets on the front end and two brackets on each rear side of the chassis. The brackets are indicated with a sticker.

These securing points and its location have been designed and successfully tested according to ISO 7176-19 – 2008.

The angle of the straps should be around 45° to the horizontal plane. This is to have maximum effect in vertical and horizontal direction.





The straps must be connected to the vehicle at suitable anchor points. Make sure that the tire pressure is at the recommended level, so the straps can have maximum effect. Make sure the straps are tightened to maintain optimal security.




WARNING

- Poor fixations of the wheelchair in a vehicle might cause damage to the vehicle itself, the wheelchair or the passengers inside the vehicle while driving. Not using a car safety belt while sitting in a wheelchair might lead to serious injuries in case of an accident.
- Alterations or substitutions should not be made to the wheelchair securement points or to structural- and frame parts or components without consulting the wheelchair manufacturer.


18.1.2 Safety belt

If the user is transported in his wheelchair, it is necessary to use a car safety belt to secure the wheelchair user.

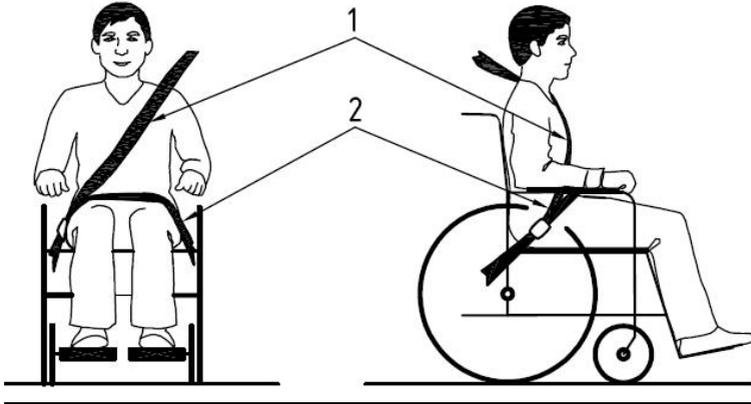


Positioning of the car safety belts for wheelchair users.

The wheelchair has been crash tested using a Dahl heavy duty tie-down belt, model 501780 or 501781, and a 3-point occupant restraint (Dahl part no: 500984). We advise you to use a similar system or a system that is equally specified. It is very important to use the safety belt at the right angles according to the wheelchair user. The angle for the pelvis part (2) of the safety belt must be at the angle of 30–75° with the horizontal plane. (See picture below). Also, the side angle should stay between the vertical plane to maximum of 15° angle with the vertical plane. (See picture below).

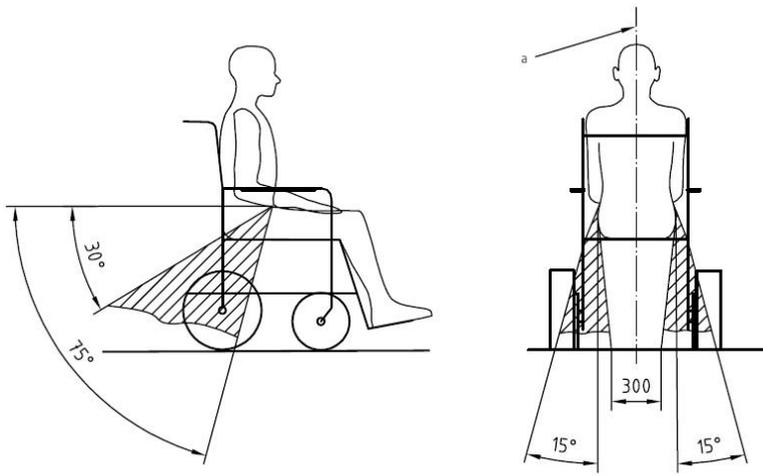

Optimal angles for a safety belt used by the wheelchair user

The shoulder part (1) of the safety belt should be positioned according to the figure below.

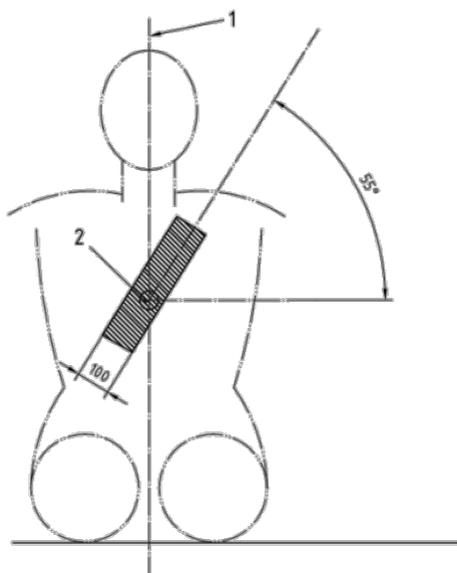

Shoulder safety belt positioning



NOTE

Please obtain the following points for an optimal personal safety of the wheelchair user:


- the pelvic belt should be worn low across the front of the pelvis, so that the angle of the pelvic belt is within the preferred zone of 30° to 75° to the horizontal, as shown in figure above.
- a steeper (greater) angle within the preferred zone is desirable.
- belt restraints should not be held away from the body by wheelchair components or parts, such as the wheelchair armrests or wheels, along with an illustration similar to that of the figure shown above.
- upper torso belts should fit over the shoulder and across the chest, as illustrated in figure of the shoulder safety belt positioning.
- belt restraints should be adjusted as tightly as possible, consistent with



NOTE

user comfort.

- belt webbing should not be twisted when in use.

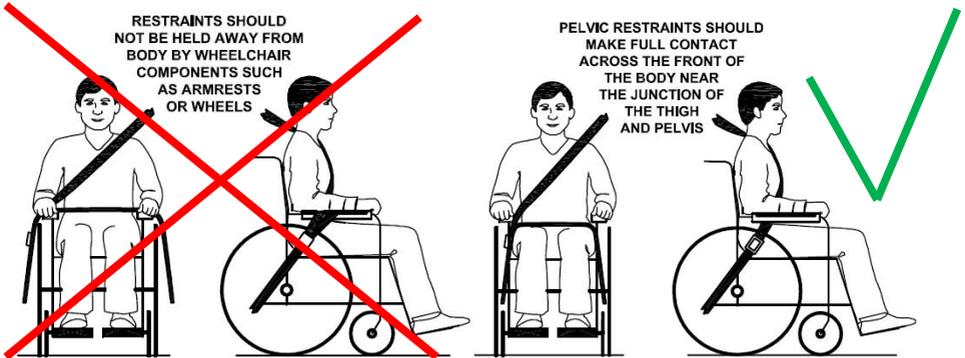

Picture of improper belt fit

Picture of proper belt fit



NOTE

Please, make sure the following conditions are fulfilled to obtain a safe transportation:

- Whenever possible the occupied wheelchair shall be located in a forward-facing configuration and secured by the tie downs in accordance with the WTORS (wheelchair tie down and occupant-restraint system) manufacturer's instructions.
- This wheelchair is suitable for use in vehicles and has met the performance requirements for travelling forwards-facing in frontal impact conditions. Its use in other configurations within a vehicle has not been tested.
- The wheelchair has been dynamically tested in a forward-facing orientation with the ATD (anthropomorphic test device) restrained by both pelvic and upper torso belts.



NOTE

- Both pelvic and upper torso belts should be used to reduce the possibility of head and chest impacts with vehicle components.
- When possible, other auxiliary wheelchair equipment should be either secured to the wheelchair or removed from the wheelchair and secured in the vehicle during transit, so that it does not break free and cause injury to vehicle occupants in the event of a collision.
- Positioning supports should not be relied on for occupant restraint in a moving vehicle unless they are labeled as being in accordance with the requirements specified in ISO 7176-19 – 2008.
- The wheelchair should be inspected by a manufacturer's representative before reuse following involvement in any type of vehicle impact.
- Alterations or substitutions should not be made to the wheelchair securement points or to structural and frame parts or components without consulting the manufacturer.
- Only use "gelled electrolyte" batteries on powered wheelchairs when used in a car.

18.2 Transportation using Dahl Docking station

Evo Lectus Low Rider (EVO-LTS-LR) has also been crash tested using a Dahl docking station tie down system according to ISO 7176-19 – 2008 and 10542-1:2012 SWM, where the wheelchair is facing forward in driving direction (driving direction like the driver seat).



Evo Lectus Low Rider (EVO-LTS-LR) crash test using Dahl Docking station.

The locking of the wheelchair into the Dahl Docking station makes it much easier to lock down the wheelchair for occupied transportation. It can be used also for wheelchair users who want to drive the car by themselves. The system is self-locking and can be released by pushing a button. The locking device will open up for a certain time to make the un-docking possible.



WARNING

The Dahl Docking station is only allowed to build into a vehicle by trained and authorized staff of a registered car adaptation company. For ordering the Dahl Docking and its accessories, please contact Dahl Engineering in Denmark for further details. You can find Dahl at www.dahlengineering.dk

18.2.1 Mounting of the Dahl locking adapter on the wheelchair


The EVO chassis can be equipped with a Dahl docking plate underneath the battery box frame of the chassis.



EVO chassis with Dahl Docking plate mounted

For detailed information about the Dahl Docking system, please visit the homepage: www.dahlengineering.dk

To fit the Dahl docking plate, Dahl has created a special kit for EVO chassis which included the special Dahl nut plates and the spacers for the battery box of EVO to level the batteries. This kit is available under Dahl part no: 503194

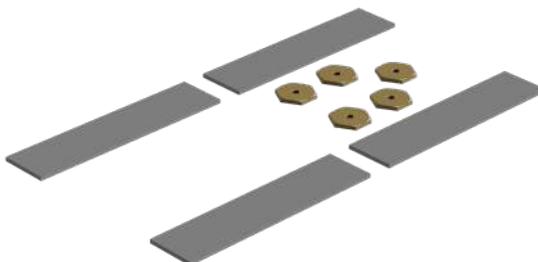

503194 EVO/Dahl mounting nut and spacers



WARNING


The Dahl Docking station is only allowed to build in to a vehicle by trained and authorized staff of a registered car adaptation company. For ordering the Dahl Docking and its accessories, please contact Dahl Engineering in Denmark for further details. You can find Dahl at www.dahlengineering.dk

The EVO chassis has dedicated holes in the chassis where the Dahl Docking plate can be mounted on.



Dedicated holes for mounting Dahl Docking plate

1. Remove the batteries from the EVO Chassis and put the 5 special Dahl nut plates into the dedicated mounting holes from the inside of the battery box.

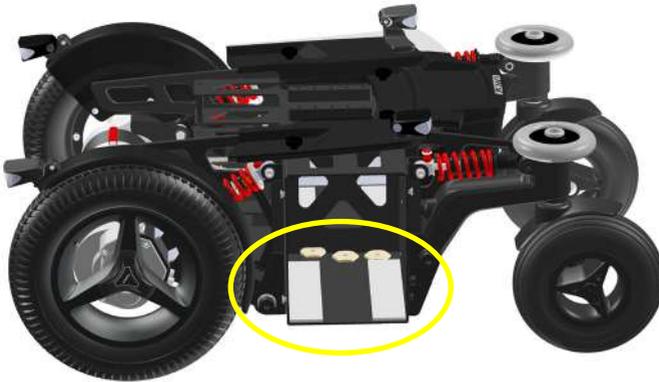

2. Two plastic spacers are to be placed in every battery box on the floor. Best is to fix them with some double-sided tape.
3. Now take the Dahl spacer (Dahl part no: 500673, docking plate (Dahl part no: 500561 and 5 special Dahl high grade steel (14.9) Torx bolts (Dahl part no: 502800) to mount the Dahl docking plate on to the EVO chassis.



NOTE

The special Dahl high grade Torx bolts (Dahl part no: 502800) only come in one length which often is too long. They need to be cut into the right length by the authorized engineer to fit the locking plate properly without damaging the batteries.



Mounting the Dahl docking plate on to the EVO chassis

4. After cutting the bolts to the right length, Loctite 222 needs to be added on to the thread to secure the bolts.
5. The five Torx bolts shall be tightened with a torque wrench to the preset torque of 20-24 Nm.
6. Place the batteries back into the chassis and connect them to the electronics.

Now the EVO chassis is ready to be docked into the Dahl Docking station. The mounting of the Dahl docking station into your vehicle shall only be executed by an authorized car adaptation company. They will get the right support and information from Dahl Engineering how to mount the docking station in to the designated vehicle.



WARNING

The Dahl Docking station is only allowed to build in to a vehicle by trained and authorized staff of a registered car adaptation company. For ordering the Dahl Docking and its accessories, please contact Dahl Engineering in Denmark for further details. You can find Dahl at www.dahlengineering.dk




Dahl docking station



Dahl docking station mounted on the floor



Docking station and docking plate on chassis

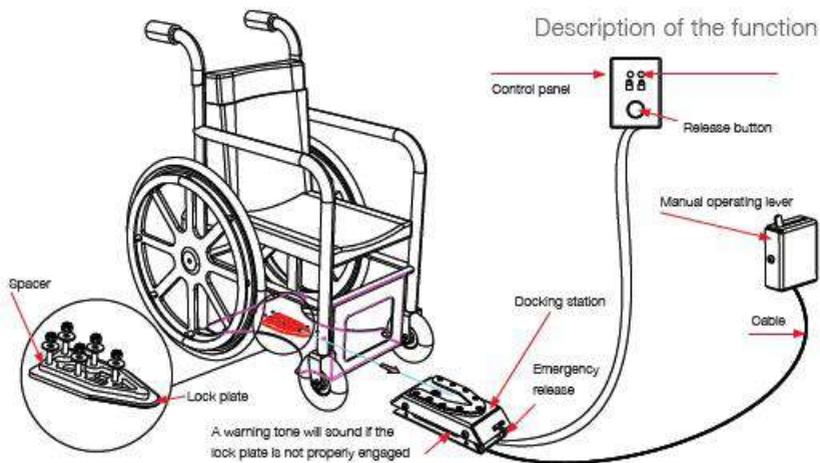

18.2.2 Locking procedure:

First, lift up the support wheels of the Evo Lectus Low Rider (EVO-LTS-LR). This is in order to avoid a collision with the ramp. Now drive the wheelchair slowly into the vehicle and make sure you centre your wheelchair in the middle of the docking module. If being well positioned the locking system will also guide the wheelchair into the docking station. Keep in slowly driving until you feel the wheelchair is hitting the end position in the docking station. At the same time you will hear a clicking sound. The wheelchair is now locked in to the docking station. the light on the control panel will light up the LED showing the wheelchair is locked in correctly. Now switch the wheelchair off.



WARNING

If the wheelchair is not centered correctly, it might not be possible to lock in top the docking station. In that case, retry by driving a bit backwards and re-center the wheelchair. try once more until you hear the clicking sound and you see the locked sign LED on.

After the wheelchair is locked in, put the car safety belt on according to the instruction in chapter 19.3.



WARNING

Do not forget to put the car safety belts on before driving in the vehicle. This on order to avoid dangerous situations and personal- or wheelchair damage.

18.2.3 Unlocking procedure:

To unlock the wheelchair, first open up the car safety belt. Then switch on the wheelchair and switch to drive mode. Now push the release button of the Dahl Docking station. You will hear a firm click. The locking bolt is now retracted and the wheelchair can drive in reverse direction out of the Docking station.




NOTE

After pushing the release button of the Dahl Docking station, the locking bolt is retracted for a certain period of time. After that time, the bolt will lift up again and lock the Docking station. Make sure you drive your wheelchair out of the Docking station in this time window of the unlocked position. If not, you have to push the release button one more time.

18.2.4 Manually unlocking in case of electric failure or accident:

The Dahl Docking station can be unlocked manually in case of an emergency or if the electric unlocking is failing.

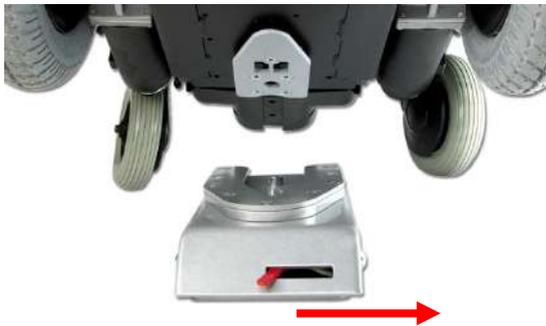

To unlock the docking station manually, the red lever needs to be pulled to the right. This retracts the locking bolt manually so the wheelchair can be released out of the docking station.




WARNING

In case of a failure of the docking station, contact your local car adaptation company who has built in the device into your vehicle. Only authorized and trained staff is allowed to work on the docking device.


18.2.5 Safety belt

If the user is transported in his wheelchair, it is necessary to use a car safety belt to secure the wheelchair user.

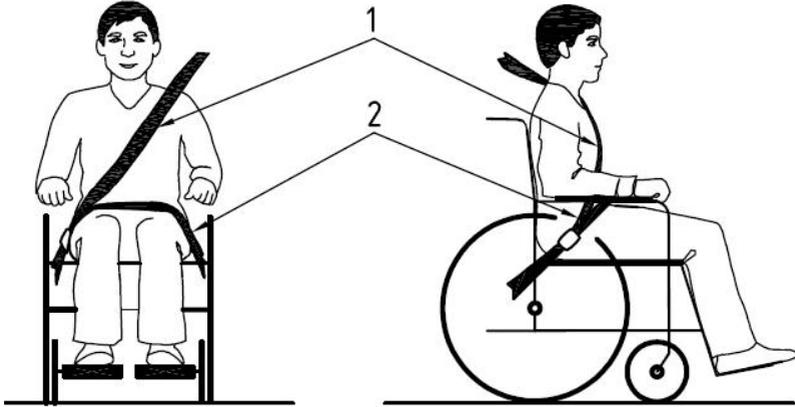


Positioning of the car safety belts for wheelchair users

The wheelchair has been crash tested using a Dahl 3-point occupant safety belt, model 500984. We advise you to use a similar system or a system that is equally specified. It is very important to use the safety belt at the right angles according to the wheelchair user. The angle for the pelvis part (2) of the safety belt must be at the angle of 30–75° with the horizontal plane. (See picture below). Also, the side angle should stay between the vertical plane to maximum of 15° angle with the vertical plane. (See picture below).

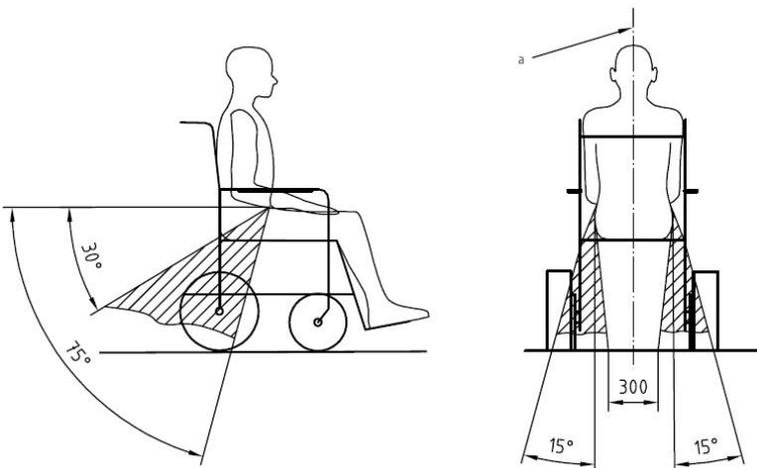

Optimal angles for a safety belt used by the wheelchair user

The shoulder part (1) of the safety belt should be positioned according to the figure below.

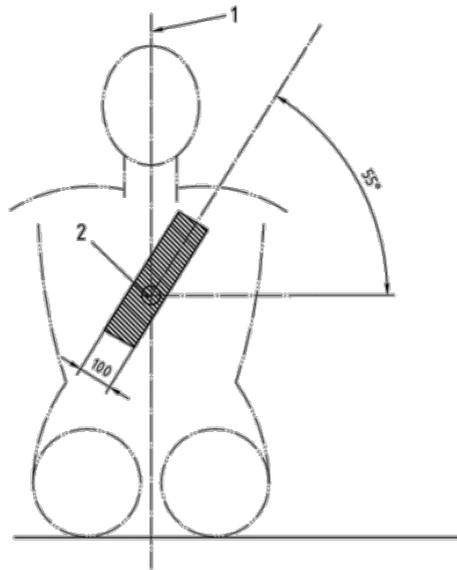


Shoulder safety belt positioning



NOTE

Please obtain the following points for an optimal personal safety of the wheelchair user:

- the pelvic belt should be worn low across the front of the pelvis, so that the angle of the pelvic belt is within the preferred zone of 30° to 75° to the horizontal, as shown in figure above.
- a steeper (greater) angle within the preferred zone is desirable.
- belt restraints should not be held away from the body by wheelchair components or parts, such as the wheelchair armrests or wheels, along with an illustration similar to that of the figure shown above.
- upper torso belts should fit over the shoulder and across the chest, as illustrated in figure of the shoulder safety belt positioning.
- belt restraints should be adjusted as tightly as possible, consistent with user comfort.
- belt webbing should not be twisted when in use.

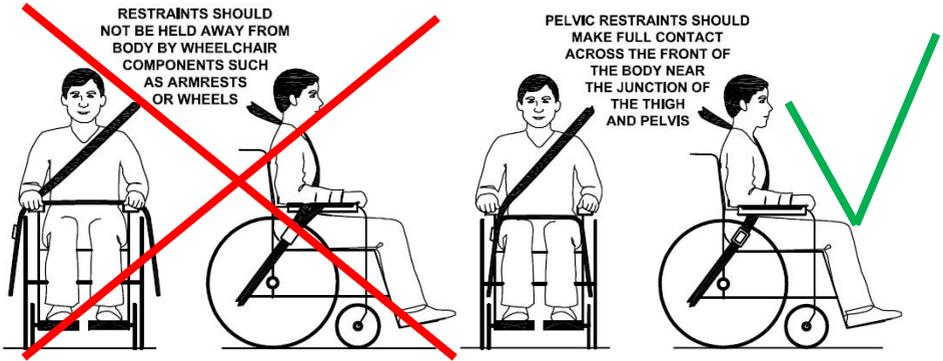

Picture of improper belt fit

Picture of proper belt fit



NOTE

Please, make sure the following conditions are fulfilled to obtain a safe transportation:

- Whenever possible the occupied wheelchair shall be located in a forward-facing configuration and secured by the tie downs in accordance with the WTORS (wheelchair tie down and occupant-restraint system) manufacturer's instructions.
- This wheelchair is suitable for use in vehicles and has met the performance requirements for travelling forwards-facing in frontal impact conditions. Its use in other configurations within a vehicle has not been tested.
- The wheelchair has been dynamically tested in a forward-facing orientation with the ATD (anthropomorphic test device) restrained by both pelvic and upper torso belts.
- Both pelvic and upper torso belts should be used to reduce the possibility of head and chest impacts with vehicle components.
- When possible, other auxiliary wheelchair equipment should be either secured to the wheelchair or removed from the wheelchair and secured in the vehicle during transit, so that it does not break free and cause injury to vehicle occupants in the event of a collision.
- Positioning supports should not be relied on for occupant restraint in a moving vehicle unless they are labeled as being in accordance with the requirements specified in ISO 7176-19 – 2008.
- The wheelchair should be inspected by a manufacturer's representative



NOTE

before reuse following involvement in any type of vehicle impact.

18.3 Transportation on an airplane


When transporting your wheelchair by air, you should primarily pay attention to the following three things:

18.3.1 Batteries

Gel batteries: In most cases, they do not need to be removed from the wheelchair. The batteries only need to be disconnected from the wheelchair. To do this simply unplug the main fuse in the rear of the chassis.



Position of the main fuse

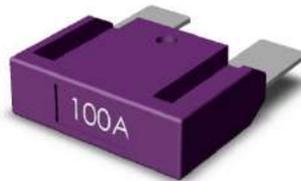

Main fuse

Acid batteries: Most airlines require that batteries be removed from the wheelchair and transported in special boxes that the airline may provide.

When transported by air, the wheelchair will be put with other goods in a confined space. Therefore, it is important to take preventive action to minimize transport damage to the wheelchair. Cover the control panel with soft, shock-absorbing material (foam plastic or similar) and fold it in towards the back rest. Protect other protruding objects in a similar manner. Tape any loose cables to the seat or covers.

18.3.2 The wheelchair's dimensions and weight

How much the wheelchair weighs and how large it is are important, depending on the type of airplane on which the wheelchair is to be transported. The smaller the airplane is, the smaller the wheelchair may be/weight and vice versa. Always check with the airline what rules apply.

19. Maintenance and repairs

The user and attendant must take care of some maintenance, service and occasionally fault-finding activities. Other activities as described in this paragraph should be carried out under supervision of your authorized dealer.

19.1 Battery charging

This wheelchair is provided with two maintenance-free batteries. During normal use, the batteries must be charged every day. It is most convenient to make it a daily practice to charge the wheelchair during the night.



NOTE

- Only charge in a well-ventilated room with no sources of open fire.
- Turn off the control unit before charging.
- Make sure the charging cable is not causing crashes of people.
- When the charger is disconnected from the wheelchair, also disconnect the charger from the mains.
- Place the charger in a place where it can radiate its heat freely during charging.

After having taken care of these precautions, charge the batteries by plugging in the charger in the rear of the control unit first. Plug in the charger in the mains secondly. Read the manual of your charger carefully for any other precautions and user prescriptions. When the wheelchair is not used over a longer period, recharge the batteries every four weeks to keep the batteries in good condition. If the batteries are not charged regularly, the remaining capacity will quickly drop.

19.2 Short-term storage

For the charging process to produce a battery with good capacity, the temperature in the storage room should not be lower than +5 degrees. If it is stored at a temperature below +5 degrees, there is a higher risk that the battery has not been fully charged when it comes to be used and also a higher risk of corrosion.

19.3 Long-term storage

The battery may be stored in an unheated room, but it should be charged at least once a month for maintenance purposes.



NOTE

- When the wheelchair is to be stored for a long term, we advise you to disconnect the batteries from the wheelchair. This way the batteries will hold their energy for a longer period.
- When re-using the wheelchair, the batteries will be installed and fully charged.
- Ask your local authorized supplier to store and maintain the batteries if they are not used for a long period (more than two months).
- Please note that a battery discharges itself and that a discharged battery can burst when it is cold. If the wheelchair is to be stored unused for an extended period, the batteries must always be charged once a month to avoid them being damaged.
- The wheelchair must not be stored in areas subject to condensation (steam or moisture on surfaces), for example utility rooms or similar.
- The wheelchair may be stored in an unheated room. From the point of view of corrosion, it is best for the room to be a few degrees warmer than the surroundings as this keeps the room drier.
- If the wheelchair is fitted with acid batteries, the acid level should be checked regularly. If the wheelchair is fitted with gel batteries, the liquid level does not need to be checked.
- The life of the batteries depends entirely on regular charging.

19.4 Tools

The wheelchair comes with a tool kit to be able to adjust most settings.



NOTE

- Some repairs may require tools other than those supplied with the wheelchair.
- Any unauthorized alterations to the wheelchair and its systems may lead to an increased risk of accident.
- All alterations to and interventions in the wheelchair's vital systems must be performed by an authorized service engineer. In case of doubt, always contact an authorized service engineer.



WARNING

- The main fuse must always be removed when batteries are replaced. Always switch off the power supply to the control panel before interrupting the power with the main fuse.
- Damage caused by self-servicing or servicing by unauthorized personnel cannot be claimed under warranty!
- If you have any doubt in the capability of yourself or the service engineer, please contact your local authorized supplier to help you.

19.5 Wheels and tires

Check at regular intervals that the wheelchair's tires have the correct tire pressure.

Check regularly that the tire pressure is okay. We suggest to check the tire pressure at least every 4 weeks.

Type of tire	Tire size	Recommended pressure	Max. pressure
Drive wheel tire	3.00-8	43.5 PSI, 3 Bar, 300 Kpa	50.7 PSI, 3.5 Bar, 350 Kpa
Rear caster tire	2.80-2.50-4	29.0 PSI, 2 Bar, 200 Kpa	36.2 PSI, 2.5 Bar, 250 Kpa





WARNING

An incorrect tire pressure may result in lower stability and maneuverability. Too low tire pressure also results in abnormal wear and shorter driving range.

19.5.1 Puncture repair

Since the wheelchair is rather heavy, it is recommended to let your authorized supplier repair eventual tire punctures. First lift the wheelchair so that the punctured tire is free from the ground. Both drive wheel and rear caster tires can be taken off by loosening the bolts which hold the wheels on to the wheelchair. The drive wheels should be taken off from the motor hub by first taking away the cover plate **(A)** and then loosening the 3 bolts **(B)**.

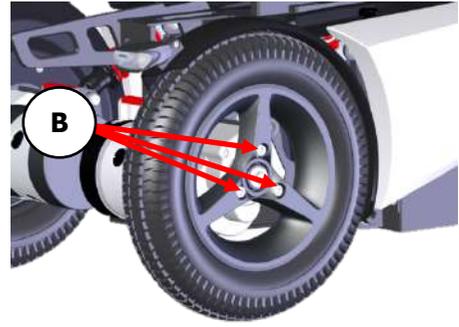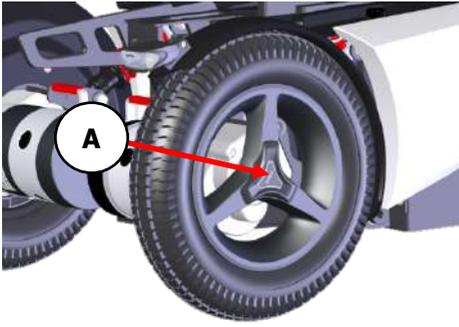


WARNING

Do not loosen the central hub bolt to remove the drive wheel.



After taking the wheels of the wheelchair, the rim can be split. The tire is then available for repair. The inner tubes of the tires can be repaired according to

the description on the tire puncture repair kit that you use. It is however recommended to renew the inner tube at all times when the tube has a puncture.

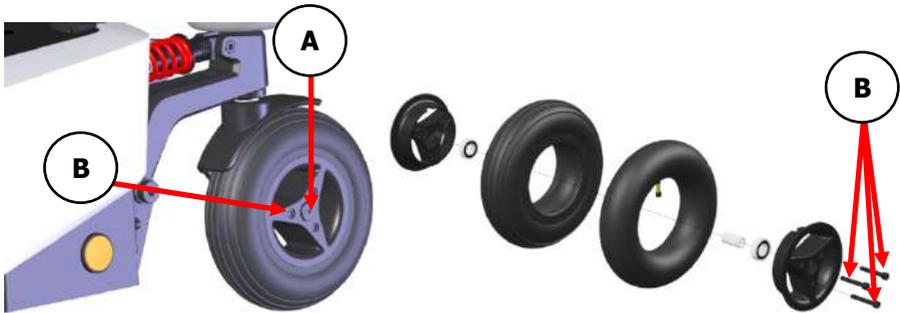

The rear casters should be taken off from the axle by loosening the center bolt (A). The tire can be taken off by loosening the 3 bolts (B) and splitting the rim.

19.6 Cleaning

Regular care and maintenance will prevent unnecessary wear and damage to your wheelchair. The following is general advice recommended by KARMA. For severe soiling of the upholstery or damage to the surface finish, contact KARMA or your local authorized supplier for information.

19.6.1 Upholstery, cloth/airmesh

For normal cleaning, wash the upholstery with hand warm water and a mild nonabrasive soap. Use a soft cloth or brush. Before the surface dries, wipe off any water/soap residues with a clean, dry cloth. This procedure may be repeated to remove stubborn dirt or stains.

If necessary, the cover may be removed before cleaning. See also the washing instructions on the label of the upholstery materials.

19.6.2 Metal surfaces

For normal cleaning it is best to use a soft cloth/sponge, hand warm water and a mild detergent. Wipe down carefully with a cloth and water, and dry off. Remove scuff marks from semi-matt surfaces with soft wax (follow manufacturer's instructions).

Remove scuff marks and scratches from shiny surfaces using car polish, either liquid or paste. After polishing, apply soft car wax to restore the original surface gloss.

19.6.3 Plastic covers

For normal cleaning, wash plastic surfaces with a soft cloth, mild detergent and hand warm water. Rinse thoroughly and dry with a soft cloth. Do not use solvents or abrasive kitchen cleaners.




WARNING

- Never use aggressive chemical cleaner or cleaning fluids. These will damage the surface and structure of the material.
- Never use a sponge with a hard surface. This will damage the surface and structure of the material.
- Never use a high-pressure water hose or steam cleaner. This will damage the surface and structure of the material and could cause electronic failure.

19.7 Brake release, freewheel mode

Check regularly, approximately once a month, that the brake release and the freewheel levers are working properly.

When the brakes are released, it should not be possible to drive the wheelchair.

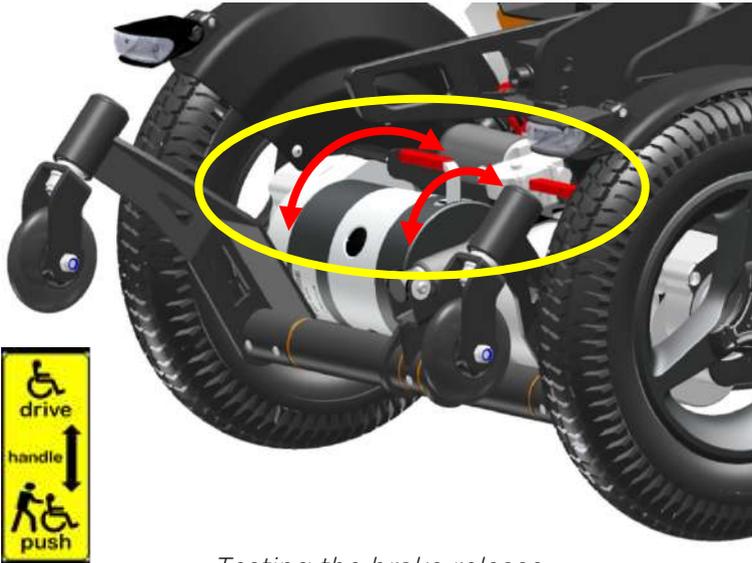

Testing the brake release


19.8 Battery replacement

- Step 1: Place the wheelchair on a level surface and, if possible, raise the seat lift for better access.
- Step 2: Switch off the power supply using the ON/OFF key on the control panel and remove the main fuse at the rear of the chassis.
- Step 3: Undo the knob holding the battery cover locked.
- Step 4: Lift the cover until you reach the end stop.
- Step 5: Pull the cover horizontally away from the chassis.
- Step 6: Pull the batteries almost out and disconnect the battery connections.
- Step 7: Replace the batteries
- Step 8: Reconnect the batteries according to the schematic which is place on the inside of the battery covers.
- Step 9: Place the batteries inside the battery box. Make sure the cables are not jammed between the battery and the chassis!
- Step 10: Put the battery covers back into place.
- Step 11: Secure the battery covers with the hand screw.



WARNING

- If you are not capable of replacing the batteries by yourself or you don't feel comfortable doing it, please contact your local authorized supplier for help.
- Damage on the wheelchair because of a not proper repair or replacement is not covered by our product warranty.

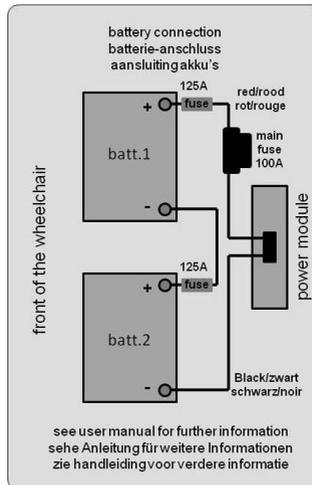

Battery connection sticker



WARNING

- Damage on the wheelchair because of a not proper repair or replacement is not covered by our product warranty.
- Batteries are classified as chemical waste and need to be disposed according to the local regulations for chemical waste.

19.9 Replacing the main fuse

To replace the main fuse, follow the next steps:

Step 1: Go to the rear end cover of the chassis

Step 2: Pull off the rubber cover of the fuse holder.


Step 3: Pull out the main fuse.

Step 4: Place the new fuse into the holder and press it tight.

Step 5: Place the rubber cover on to the fuse holder.



Place of the main fuse

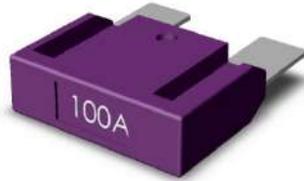

Main fuse



WARNING

- Only use original and official spare part fuse from KARMA. Other fuses might cause errors again or even fire.
- Wear protective gear when replacing the fuse, like safety goggles and hand gloves.
- If you are not capable of replacing the batteries by yourself or you don't feel comfortable doing it, please contact your local authorized supplier for help.
- Damage on the wheelchair as a result of a not proper repair or replacement is not covered by our product warranty.

20. Refurbishment and re-use of the product.

This wheelchair is suitable for refurbishment and re-use. This means that, if the wheelchair is not used anymore by the first user, it can be refurbished to fit another user. Should you not be able to use the wheelchair any longer, we strongly recommend you contact your local authorized supplier to have it picked up for refurbishment and re-use.



WARNING

- The refurbishment of the wheelchair is only allowed to be executed by an authorized supplier.
- If the wheelchair is refurbished by a non-authorized supplier or institute, KARMA Medical cannot be held responsible for this product, and all warranty claims will be voided.



NOTE

The wheelchair will be refurbished according to a refurbishment guideline of KARMA. This includes the replacement of all upholstery parts, a total disinfection of the product and a complete technical check of the wheelchair and its accessories.

21. Disposal of the product

When disposing of the used wheelchair, you need to follow the local legal regulations for disposals.

We strongly recommend you contact your local authorized supplier to take care of the disposal of your wheelchair.



WARNING

Batteries are classified as chemical waste and need to be disposed according to the local regulations for chemical waste.

22. Troubleshooting

The following troubleshooting guide describes a number of faults and events which may occur when you use your wheelchair, together with suggested remedies. Note that this guide cannot describe all the problems and events which may occur, and you should always contact your local authorized supplier or KARMA in case of doubt.

Event	Possible cause	Remedy
the wheelchair does not start up	Batteries discharged.	charge the batteries
	The cable connection of the control panel has come loose	reconnect the cable
	main fuse is defect	replace main fuse CHECK FIRST!!! see page 105
wheelchair doesn't drive	charge still connected	disconnect charger
	brake release activated	de-activate brake release
	wheelchair locked	unlock the wheelchair
the wheelchair switches itself on after a certain while	the energy saving mode has been activated	restart wheelchair using the on/off button

Event	Possible cause	Remedy
the wheelchair stops whilst being driven	a cable connection of the R-net system has come loose	check all R-net connections and restart
	main fuse has triggered	replace main fuse CHECK FIRST!!! see page 105
the wheelchair only drive at reduced speed	a speed reducing inhibit is activated	move the seat into a position where max. speed is allowed.
	Gyro has been disconnected	re-connect gyro NEED SERVICE!!
certain powered seat function is not displayed in menu	cable connection of seat function in disconnected	call for service
	seat function motor defect	call for service
wheelchair cannot be charged	main fuse disconnected	re-install main fuse
	main fuse has triggered	replace main fuse CHECK FIRST!!! see page 105
	connection between charger and joystick module not good	check connection call for service

Note that this guide cannot describe all the problems and events which may occur and you should always contact your local authorized supplier or KARMA in case of doubt.

22.1 Diagnostics R-net LCD

When an error or a fault occurs in the wheelchair's electronics, information on it is displayed in the control panel's display. This information can then be used to diagnose where the error/fault occurred and its cause.

Troubleshooting and repairs must always be performed by authorized personnel with good knowledge of the wheelchair's electronics.

Diagnostic screens

When the control system's integrated protection circuits have been triggered so that the control system can no longer operate the wheelchair, a diagnostic screen is displayed in the control panel's display.



This indicates a system fault, i.e. R-net has detected a problem somewhere in the wheelchair's electrical system.



NOTE

If the fault is in a module that is not currently being used, it may still be possible to drive the wheelchair, but the diagnostic screen is displayed occasionally.

Switch off the wheelchair and leave it off for a few minutes. Then restart the wheelchair. If the fault persists, you must switch off the wheelchair and contact your service contacts. Write down the information displayed in plain text in the control panel's display and pass it on to your local authorized supplier's service contact.



WARNING

Diagnostics should only be performed by authorized persons with sound knowledge of the wheelchair's electronic control system. Incorrect or poorly performed repair works may make it dangerous to use the wheelchair. KARMA accepts no liability for any personal injury or damage to the wheelchair and its surroundings that occurs because incorrect or poorly performed repair work. If the wheelchair is refurbished by a non-authorized supplier or institute, KARMA Medical cannot be held responsible for this product, and all warranty claims will be voided.

23. Safety information

During normal use, if the circuit breaker trips, please be sure to handle it properly as follows:



CAUTION

Important safety instructions about the circuit breaker:

- Once the circuit breaker trips, you must wait 3 minutes for the system to cool down before pressing the reset button to reset it.
- If the circuit breaker trips twice repeatedly while in operation, **DO NOT** press the reset button again. Seek assistance to move your product to a safe and flat place and contact your customer service technician for further assistance.

Safety knowledge:

- When the circuit breaker trips, it indicates that your product may have encountered an abnormal situation under special operating conditions, such as climbing a slope.
- If the electronic/electrical components overheat due to prolonged climbing, the circuit breaker will trip immediately to activate the product's safety mechanism.
- Once tripped, if you forcibly press the reset button more than twice, it may cause the electronic/electrical components to fail, leading to safety issues with the product.



WARNING

If the circuit breaker trips twice repeatedly, it indicates that the product system is not suitable for the current operating conditions. Stop using the product immediately and contact your customer service technician for further assistance. KARMA will not be responsible for any product damage or personal injury resulting from such misuse.

24. Technical specifications



Transportation size

**NOTE**

The available features, specifications, and configurations may vary depending on the country/region where you purchase the product. Contact your local sales representative for details.

Product Model	Evo Lectus Low Rider (EVO-LTS-LR)	
Seating System	Minimum	Maximum
Nominal seat width (mm/in) ¹	420 / 17	520 / 21
Nominal seat depth (mm/in) ²	400 / 16	600 / 24
Backrest height without cushion (mm)	565	725
Backrest height with cushion (mm)	510	670
Headrest height above seat (mm)	730	890
Armrest to seat distance without cushion (mm)	255	375
Armrest to seat distance with cushion (mm)	180	300
Front location of armrest structure (mm)	0	410
Seat surface height at front edge without cushion (mm)	415	865
Seat surface height at front edge with cushion (mm)	480	930
Footrest to seat distance	180	555

Product Model	Evo Lectus Low Rider (EVO-LTS-LR)	
without cushion (mm)		
Footrest to seat distance with cushion (mm)	255	630
Effective seat width (mm)	420	520
Effective seat depth (mm)	400	600
Seat plane angle (X°)	0	50
Backrest angle (X°)	-5	90
Seat to backrest angle (X°)	85	180
Leg to seat angle (X°)	85	180
Driving Characteristics	Minimum	Maximum
Drive wheel size	3.00 - 8 (14")	
Rear caster size	2.80/2.50 - 4 (9")	
Overall length with legrest (mm)	-	1200
Overall width (mm)	610	660
Overall height (mm)	1115	-
Folded length (mm)	1150	-
Folded width (mm)	610	-
Folded height (mm)	745	-
Total mass (kg)	-	185
Total mass without batteries (kg)	-	140
Mass of the heaviest part (kg)	-	135
Maximum user weight (kg)	-	136
Drive range (km) ³	-	54

Product Model	Evo Lectus Low Rider (EVO-LTS-LR)	
Maximum speed forward (km)	-	12
Minimum braking distance from max speed (mm)	2000	-
Obstacle climbing (mm)	-	70
Ground clearance (mm)	70	-
Minimum turning radius (mm)	750	-
Minimum turning radius without user (mm)	750	-
Reversing width (mm)	750	-
Static stability downhill (X°)	9	
Static stability uphill (X°)	9	
Static stability sideways (X°)	9	
Dynamic stability uphill (X°)	6	
Ability to climb rated slope (X°) ³	12	
Electrical System		
Motor power (W)	320	
Battery capacity (Ah)	80*2	
Charger output current (A)	8	
Battery Compartment (L x W x H) (mm)	265 x 175 x 235 (Single Compartment)	
<p>1. Nominal seat width is measured the width of seat cushion at 120 mm in front of the backrest. This value is mainly used in the product ordering process.</p> <p>2. Nominal seat depth is measured from the front end of the seat cushion to the back cushion. This value is mainly used in the product</p>		

ordering process.

3. Drive range/Ability to climb rated slope are estimated based on the following conditions: 20°C–35°C, 136 kg occupant, brand new fully charged batteries and driving on the flat road.

- Evo Lectus Low Rider (EVO-LTS-LR) satisfies the requirements according to EN 12184 and the maximum occupant mass is 136 kg.
- The actual product specifications differ from the data in the table by ± 1 cm ± 0.5 kg.
- The actual product specifications may vary according to different configurations.
- KARMA reserves the right to modify information herein without further notice.
- If you want to know more about the measurement methods of wheelchair specifications, please scan the QR code to read the instructions on the KARMA website.



The wheelchair conforms to the following standards:

- a) requirements and test methods for static, impact and fatigue strengths (ISO 7176-8)
- b) power and control systems for electric wheelchairs – requirements/test methods (ISO 7176-14)
- c) climatic test accordance with ISO 7176-9
- d) requirements for resistance to ignition in accordance with ISO 7176-16
- e) crash test according to ISO 7176-19 – 2008

25. Accessories

Accessories for KARMA powered wheelchairs are subject to continuous development. Every day we design new accessories to improve the flexibility of our products.

Contact your local authorized KARMA supplier for more information on the accessories which are available for your wheelchair.

Should you have a good suggestion for a new accessory, do not hesitate to contact us. Your idea might be the next new accessory!

Worldwide:

KARMA Medical
No. 2363, Sec. 2, University Rd.,
Min-Hsiung Shiang, Chia-Yi 621, Taiwan
www.karmamedical.com
globalsales@karma.com.tw

European representative:

KARMA Mobility S.L.
C/ Periodista Francisco Carantoña Dubert,
23 Bajo 33209 Gijón - Asturias (Spain)

Phone: +34 984 390 907
Email: karma@karmamobility.es
Website: www.karmamobility.es

We have a big dream

Whether it's a customized wheelchair, standing chair, general purpose chair, or another mobility aid device, each of our products is carefully designed with our customers' voices, needs, and desires in mind.

When it comes to user experiences, we strive to be more "caring," "empathetic", and "approachable".

Through our dedication and our mindfulness, we look forward to bringing more confidence, joy, and love for life to those with physical disabilities around the world.

we look forward to bringing more confidence, joy, and love for life to those with physical disabilities around the world.

KARMA Medical is continuously improving their products and accessories. Changes might take place without further notice.

karma

A Better Wheelchair, A Better Fit



KARMA MOBILITY S.L European Support Center
www.karmamobility.es
+34 984 390 907
karma@karmamobility.es

KARMA MOBILITY LTD. UK representative
www.karmamobility.co.uk
+44 845 630 3436
info@karmamobility.co.uk

KARMA MEDICAL PRODUCTS CO., LTD.
www.KarmaMedical.com
+886 5 206 6688
globalsales@karma.com.tw

(110400000916) Release Date: Feb. 2026 V.05